

*Crestal bone response to loaded zirconia
and titanium implants: a radiographic and
histometric analysis in canines*

**Corinne E. Oeschger, Dieter
D. Bosshardt, Stefan Roehling, Michael
Gahlert, David L. Cochran & Simone
F. M. Janner**

Clinical Oral Investigations

ISSN 1432-6981

Clin Oral Invest

DOI 10.1007/s00784-020-03235-2



Your article is protected by copyright and all rights are held exclusively by Springer-Verlag GmbH Germany, part of Springer Nature. This e-offprint is for personal use only and shall not be self-archived in electronic repositories. If you wish to self-archive your article, please use the accepted manuscript version for posting on your own website. You may further deposit the accepted manuscript version in any repository, provided it is only made publicly available 12 months after official publication or later and provided acknowledgement is given to the original source of publication and a link is inserted to the published article on Springer's website. The link must be accompanied by the following text: "The final publication is available at link.springer.com".



Crestal bone response to loaded zirconia and titanium implants: a radiographic and histometric analysis in canines

Corinne E. Oeschger^{1,2} · Dieter D. Bosshardt³ · Stefan Roehling^{4,5,6} · Michael Gahlert^{6,7,8} · David L. Cochran⁵ · Simone F. M. Janner^{1,5} 

Received: 14 November 2019 / Accepted: 29 January 2020
© Springer-Verlag GmbH Germany, part of Springer Nature 2020

Abstract

Objectives To evaluate the crestal bone response to a two-piece zirconia implant compared with a control titanium implant using periapical radiographs (PAs) and histometry.

Materials and methods Thirty zirconia and 30 titanium implants were placed in healed posterior mandibles of five canines. Full-ceramic single-tooth restorations were cemented after 6 weeks of healing. Three observers measured the distance between the implant shoulder and the crestal bone (DIB) at placement, loading, and harvesting after 4 or 16 weeks in function. The influence of implant material and loading time on DIB as well as the inter-observer agreement were analyzed. Additionally, histometric distance between implant shoulder and most coronal bone-to-implant contact (IS-cBIC) was compared with DIB.

Results Mean DIB values increased between 4 and 16 weeks of loading for both zirconia (from 1.66 to 2.25 mm; $P < 0.0001$) and titanium (from 1.81 to 1.95 mm; $P = 0.06$). Zirconia yielded mean IS-cBIC values of 2.18 mm and 2.48 mm ($P < 0.001$) and titanium 2.23 mm and 2.34 mm ($P = 0.27$) after 4 and 16 weeks, respectively. The raters reached an excellent intraclass correlation coefficient. PAs underestimated the bone loss on average by 0.39 mm.

Conclusions Zirconia implants showed a greater increase of DIB during early healing and function than titanium.

Clinical relevance Crestal peri-implant tissue dimensions may show more pronounced changes around two-piece zirconia implants during early healing. PAs may underestimate peri-implant bone loss.

Keywords Crestal bone · Dental implants · Osseointegration · Radiographic analysis · Zirconia implants

Introduction

Titanium implants have been successfully used for the replacement of teeth for over 40 years, since the first reports by Brånemark 1969 and Schroeder 1978 [1, 2]. Mechanical and biological stability and excellent long-term results make

titanium the gold standard as an implant material [3, 4]. Demand for metal-free implant materials has recently increased, partially due to more or less founded criticism towards titanium [5, 6] and the potential of optimal esthetic outcomes of white ceramic materials [7]. Among these, recent reports hypothesize a limited impact of bacteria from zirconia

✉ Simone F. M. Janner
simone.janner@zmk.unibe.ch

¹ Department of Oral Surgery and Stomatology, School of Dental Medicine, University of Bern, Freiburgstrasse 7, CH-3010 Bern, Switzerland

² Private Practice, Solothurn, Switzerland

³ Robert K. Schenk Laboratory of Oral Histology, School of Dental Medicine, University of Bern, Bern, Switzerland

⁴ Clinic for Oral and Cranio-Maxillofacial Surgery, Kantonsspital Aarau, Aarau, Switzerland

⁵ Department of Periodontics, University of Texas Health Science Center at San Antonio, San Antonio, TX, USA

⁶ Private Dental Clinic Prof. Gahlert and Dr. Röhling, Munich, Germany

⁷ Clinic for Oral and Cranio-Maxillofacial Surgery, Hightech Research Center, University Hospital Basel, University of Basel, Basel, Switzerland

⁸ Department for Oral Surgery, Faculty of Medicine at the Sigmund Freud University Vienna, Vienna, Austria

surfaces on the surrounding tissues [8, 9], whereas bacterial peri-implant infections are known as a main reason for the failure of titanium implants [10–12]. This may be due to a lower bacterial adhesion and plaque formation on ceramic surfaces [9, 13, 14].

Early preclinical studies on implants made of zirconium dioxide (ZrO_2 ; zirconia) appeared in the early 1990s [15], while the first clinical data were published 10 years later [16]. Then, in the last two decades, availability and use of zirconia implants increased. Preclinical data demonstrate that zirconia implants with moderately rough endosseous surface show similar osseointegration to current titanium implants [17]. Clinical studies show promising survival rates for periods of up to 5 years for currently commercially available zirconia implants [18–20]. Most implant failures occur in the first year with a survival rate of 95.6%; then, failure incidence decreases to 0.05% per year with almost constant survival curves [21].

Peri-implant tissue health is characterized by defined dimensions of soft and hard tissue [22]. On the other side, peri-implant infection is mostly associated with crestal bone loss [23] and is an important factor for implant failure [11, 12]. Peri-implantitis can be successfully treated when patients follow a regular supportive care program which results in high implant survival in the medium and long term [24]. In this context, methods for non-invasive, reliable measurement and detection of crestal bone loss are essential. Accordingly, the measurement of the distance between implant shoulder and bone crest (DIB) in periapical radiographs (PAs) is a routinely used diagnostic tool in combination with the clinical examination during the follow-up after implant therapy [25–28]. DIB measurement in PAs around titanium implants has shown good correlation when compared with the histometric measurement of the same dimension (implant shoulder to most coronal bone-to-implant contact; IS-cBIC) [28]. Zirconia implants generate significantly more artifacts than titanium in computed tomography (CT) and cone-beam CT (CBCT) scans [29, 30]. Interestingly, this material-related influence is reversed in magnetic resonance imaging (MRI) scans [31]. The current literature contains no data about the effect of implant material (zirconia vs. titanium) on DIB measurement in PAs.

The purpose of this study was to evaluate the influence of loading time and implant material on crestal bone levels around a two-piece zirconia (test) and well-documented titanium (control) implant under functional loading. Secondary objectives were the reproducibility between the observers and the comparison of the radiographic to the histometric assessment. The null hypothesis was that no statistically significant difference between test and control groups can be found in any measured parameter after 4 and 16 weeks of loading and also among the 3 observers.

Material and methods

The study was conducted in accordance with the ethical standards of current US federal regulations. The University of Texas Health Science Center at San Antonio Institutional Animal Care and Use Committee approved animal selection, management, and study protocol prior to the start of the experiment (IACUC; ID no. 13005x).

Study design

The study design has been described previously [17]. In brief, implants were placed in healed edentulous ridges 12 weeks after extraction of all mandibular premolars and first molars in five male, laboratory-bred hound dogs with mean age of 18 months (range 14–24 months). Two different implant materials were compared. The test material was a novel two-piece zirconia implant, with an endosseous diameter of 4.1 mm and endosseous length of 8 mm, featuring a machined collar of 4.8 mm diameter and 1.8 mm height (Institut Straumann AG, Basel, Switzerland). The surface of this yttria-stabilized tetragonal zirconia polycrystal implant was modified with sandblasting (large Al_2O_3 grits of 0.25–0.5 mm) and acid-etched (hydrofluoric acid) up to 0.74 μm (micro) and 1.64 μm (macro) roughness. The control was a commercially available implant with similar endosseous and collar dimensions as the test (Standard Plus Regular Neck; Institut Straumann AG). This implant made of commercially pure titanium displayed a surface with 1.26 μm (micro) and 3.14 μm (macro) roughness, obtained with a treatment identical to the control except for the etchant being a mixture of hydrochloric/sulfuric acid. Three test and 3 control implants were inserted in an alternating pattern bilaterally in the healed edentulous ridge, yielding a total of 6 implants per side. Full-ceramic, single-tooth restorations were cemented after 6 weeks of transmucosal healing, allowing for full functional loading of the implants. The crowns all had an identical outer shape and appropriate inner shape for the respective abutment type, i.e., zirconia or titanium. Both sides of the mandible were treated following the same surgical and prosthetic protocols, with the treatment of the randomly chosen first side starting 12 weeks before the second side and thus leading to two different loading periods (4 and 16 weeks, respectively) of the implants at euthanasia and harvesting (Fig. 1). Histometric procedures were performed as described previously [17].

Radiographic analysis

Periapical radiographs (PAs) were taken immediately after implant placement, after restoration, and at harvesting. For all five canines, customized radiographic stents allowing standardized x-ray projections during the experimental period were prepared. Film-holding bite blocks with a paralleling

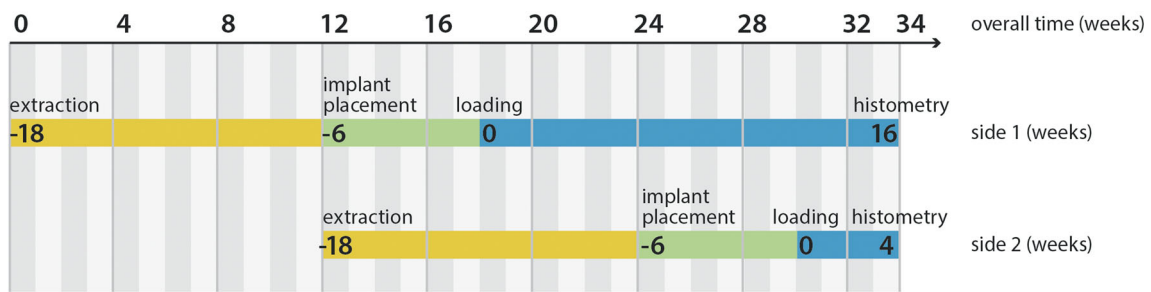


Fig. 1 Timetable of the treatment protocol

beam-guiding device (Rinn-XCP posterior; Dentsply Sirona, York, PA, USA) were adapted by means of light-curing acrylic resin engaging the canines and the second molars (Fig. 2). Each of the digital PAs was assigned a random number allowing a blinded evaluation with regard to the investigational time point. DIB measurements were performed by three observers according to the previously described method [27, 32] (Fig. 3), using digital medical imaging software (Osirix Lite Version 7.0.4; Pixmeo SARL, Bernex, Switzerland). On each PA, the vertical distance between the maximal amount of clearly visible threads of one zirconia implant was used as reference for the computer-assisted calibration. The three observers were trained oral and implant surgeons, well-experienced in dental and maxillofacial radiology. They all were calibrated by means of 10 randomly chosen PAs from the study dataset prior to the assessment of the radiographs.

Statistical analysis

The assessment of the data was performed in three consecutive steps.

Radiographic assessment (primary outcome variables)

The impact of the implant material (zirconia/titanium) on the main outcome DIB was assessed. As well, it was analyzed if the time point (placement/loading/harvesting) had a significant impact on DIB. Data was analyzed with respect to the loading period (4 or 16 weeks) at harvesting. Because of repeated measurements, all radiographic analyses were done with the help of linear mixed models.

Fig. 2 Customized X-ray holder



Homogeneity analysis of the observers (secondary outcome variables)


The inter-observer agreement (reproducibility) among the three observers was analyzed. For this purpose, inter-class correlation coefficients (ICC) were calculated and classified according to Cicchetti's grading system [33] into poor (< 0.40), fair (0.40–0.59), good (0.60–0.74), or excellent (> 0.75). In addition, the average absolute inter-observer error with its 95% confidence interval (95% CI t-interval) as well as its variability was estimated by calculating the mean of the absolute differences between all repeated measurements on the same tooth for each aspect (mesial/distal) and time point (loading/placement/harvesting) separately. This homogeneity analysis was performed chronologically as the first statistical step, in order to assess whether the three measurements of each site may be averaged for the subsequent analyses based on the agreement rate.

Histometric assessment (secondary outcome variables)

Histometric data were generated according to the previous study [17]. The outcome (IS-cBIC) was compared with the radiographic data (DIB) at harvesting using again linear mixed models. Except for the previously reported analysis of implant material and loading period [17] that serves in the comparison between histometry and PA, all data presented in this study is new.

As for the linear mixed models, the variables “implant type” (zirconia/titanium), “time point” (placement/loading/harvesting), “loading period” (4 or 16 weeks), and

Fig. 3 Schematic representation of the distance between implant shoulder and bone crest (DIB) as measured in the PA (a). Distance between implant shoulder and most coronal bone-to-implant contact IS-cBIC in an exemplary histologic specimen (b)

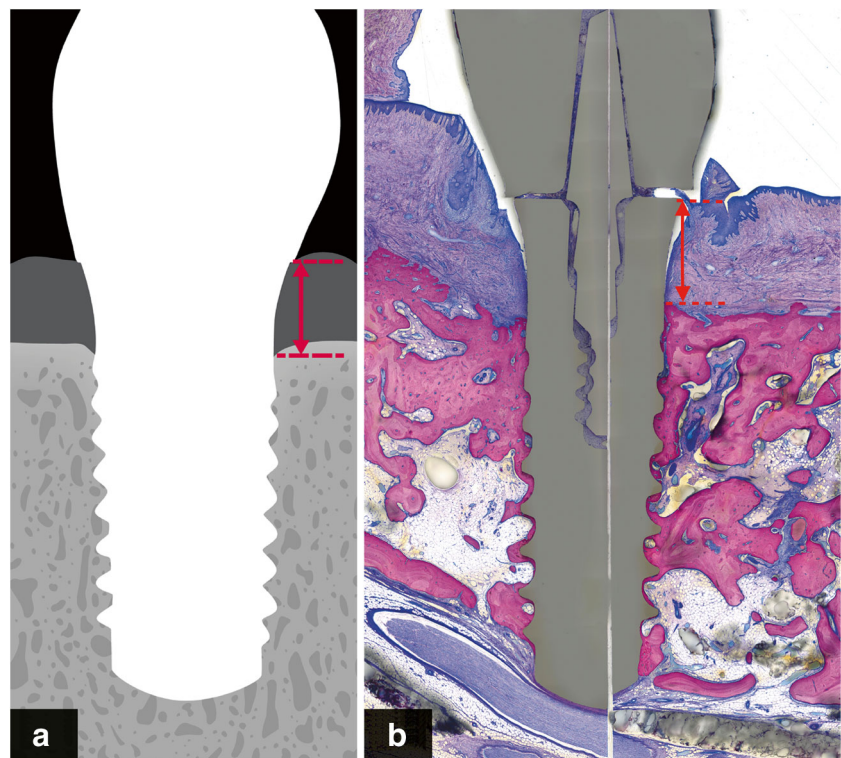

“measurement type” (radiology/histology) were always included as fixed factors whereas the variables “aspect” (mesial or distal) and “tooth-nested-in-canine” were used as random factors. A type III ANOVA F test using Satterthwaite’s correction was performed to detect global significant effects while Satterthwaite-corrected t tests were performed post hoc to detect group-wise differences. Throughout the mixed models were validated with the help of normality tests (Shapiro-Wilk) on both residuals and random effects. Also, fitted and effective values were plotted against each other to check for possible residual patterns. P values less than 0.05 were considered statistically significant. No corrections for P values and no sample size calculation were applied due to the explorative nature of this study. All analyses in this report were performed with the statistics software R, version 3.5.0 (R Development Core Team, Vienna, Austria, 2018. URL <https://www.r-project.org/>).

Results

All 60 implants and 60 restorations were still in function after 4 and 16 weeks of loading in both test and control groups. No implant loss, no implant or abutment fracture, and no chipping at the restorations could be detected. The animals remained healthy throughout the entire study time frame.

Inter-observer agreement

The inter-observer agreement was graded as “excellent” according to Cichetti [33] at all time points with intraclass correlation values (95% CI) of 0.83 (0.78–0.87) at placement, 0.86 (0.81–0.89) at loading, and 0.83 (0.77–0.87) at harvesting. The average absolute measurement error between observers was almost constantly 0.15 mm with a standard deviation of 0.15 mm (Table 1) and a maximum of 0.88 mm. This again emphasizes the strong agreement. The average measurement difference between observers was close to 0.0 mm, with an almost constant standard deviation of 0.2 mm (Table 1). Also, the overlapping confidence intervals emphasized the strong consensus. Based on the high agreement between the

Table 1 Summary of average absolute measurement errors (distances) between observers (in mm): grand mean with 95% CI, standard deviation, and range in lines 1 to 3, respectively

	Loading	Placement	Harvesting
Mesial aspect	0.15 (0.19, 0.23)	0.15 (0.19, 0.23)	0.16 (0.20, 0.24)
	0.15	0.15	0.16
	[0.01, 0.74]	[0.01, 0.60]	[0.02, 0.84]
Distal aspect	0.16 (0.20, 0.24)	0.15 (0.20, 0.24)	0.15 (0.19, 0.24)
	0.15	0.17	0.16
	[0.03, 0.81]	[0.01, 0.68]	[0.04, 0.88]

three observers, averaged values of all three observers at each time point were used for further analysis.

Radiographic assessment

The mean DIB increased for zirconia from placement (1.47 mm) to 16 weeks of loading (2.25 mm) and from 1.33 to 1.95 mm for titanium (Table 2). The implant material (zirconia/titanium) had no effect on the averaged DIB ($P = 0.33$).

The study period from placement to 16 weeks loading showed a highly significant impact on DIB ($P < 0.0001$). Hence, post hoc tests were performed to compare the different time frames. For each implant material (zirconia/titanium), DIB at each time point was compared with DIB at the other time points and then analyzed for whether there was a statistically significant difference (Table 3). For zirconia, all analyzed time frames showed statistically significant differences ($P \leq 0.004$) except between loading and harvesting after 4 weeks of loading ($P = 0.83$). For titanium, the comparisons with placement were statistically significant (all $P < 0.0001$), whereas all time point combinations after loading reached no statistical significance (all $P \geq 0.06$).

Histometric analysis and comparison to radiography

Histometric (IS-cBIC) values differed from radiographic (DIB) values at both harvesting times ($P < 0.0001$). The overall IS-cBIC was 2.31 mm, whereas the overall DIB reached 1.92 mm (Table 4 and Fig. 4). The effect of loading period was also highly significant ($P < 0.0001$), but this effect was influenced by a significant interaction with implant material ($P = 0.01$). Therefore, post hoc tests were performed to compare each group.

The loading period had a significant impact on IS-cBIC at zirconia implants, with values being higher at 16 than 4 weeks. This effect was revealed in both histometry and PA (both $P < 0.0001$). Histometry and PA thus led to the same result despite their significant difference. Opposingly, when assessing the effect of loading period on titanium implants, the group-wise comparison was close to significant in PAs ($P = 0.06$; Table 4) and far from significant at histometry ($P = 0.27$; Table 4). Similar to zirconia, titanium also yielded a high correlation between the two measurement methods at each time point (both $P < 0.0001$).

In conclusion, when comparing PAs to histometry at zirconia implants, the discrepancy between DIB and IC-cBIC

Table 3 Changes of DIB between the study time points for zirconia and titanium implants. Comparisons between all combinations of two time points, respectively

Implant material	Time frame comparison	P value
Zirconia	Placement-loading	< 0.0001
	Placement-harvesting 4 weeks	< 0.0001
	Placement-harvesting 16 weeks	< 0.0001
	Loading-harvesting 4 weeks	0.83
	Loading-harvesting 16 weeks	0.004
	Harvesting 4 weeks-harvesting 16 weeks	< 0.0001
Titanium	Placement-loading	< 0.0001
	Placement-harvesting 4 weeks	< 0.0001
	Placement-harvesting 16 weeks	< 0.0001
	Loading-harvesting 4 weeks	0.22
	Loading-harvesting 16 weeks	0.25
	Harvesting 4 weeks-harvesting 16 weeks	0.06

depended on the loading period (Table 4 and Fig. 5): the highest discrepancy was found after 4 weeks (1.66 mm vs. 2.18 mm, respectively) and the lowest at 16 weeks (2.25 mm vs. 2.48 mm). For titanium, the difference between PAs and histometry was more similar between the two time points (Table 4 and Fig. 5).

Discussion

The present study was designed to evaluate the influence of implant material (zirconia vs. titanium) and loading time (4 vs. 16 weeks) on crestal bone levels measured in PAs and histometry in a canine model. Under these experimental conditions, the zirconia implant showed a more pronounced crestal bone loss than titanium between 4 and 16 weeks of function. DIB measurements performed in the PAs reached high reproducibility. Moreover, PA tended to underestimate the distance between implant shoulder and crestal bone when compared with histometric measurements. The null hypothesis could be confirmed only for the inter-observer agreement. For all other measured parameters, there was a statistically significant difference between test and control groups after 4 and 16 weeks of loading; therefore, the null hypothesis had to be rejected.

The current literature contains a number of studies reporting high long-term survival of titanium implants such

Table 2 Mean DIB and 95% confidence interval at all time points for zirconia and titanium implants

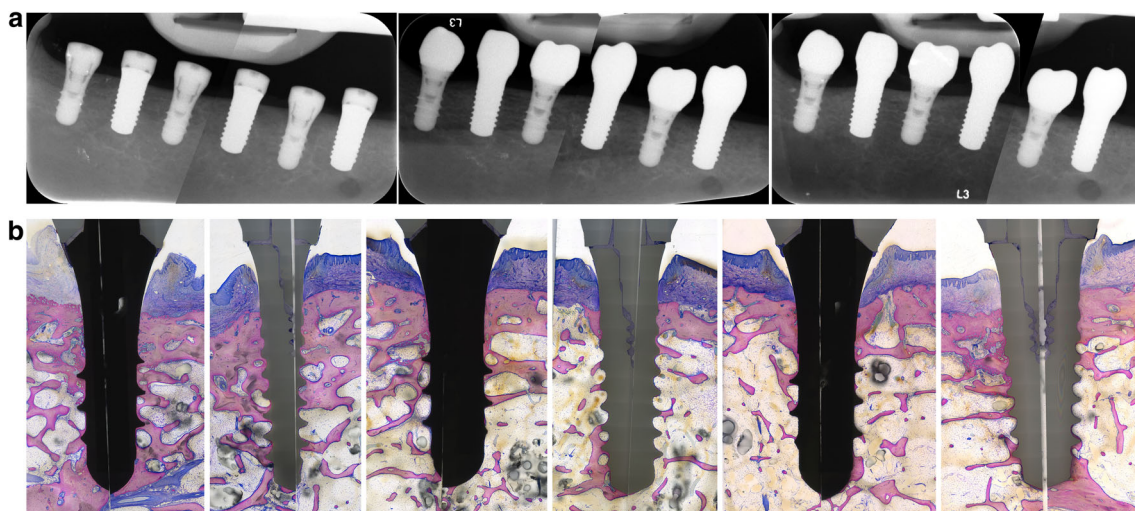
Time point	Zirconia mean DIB (mm) (95% CI)	Titanium mean DIB (mm) (95% CI)
Placement	1.47 (1.38, 1.55)	1.33 (1.22, 1.45)
Loading	1.86 (1.75, 1.98)	1.81 (1.70, 1.93)
Harvesting 4 weeks	1.66 (1.56, 1.76)	1.81 (1.65, 1.98)
Harvesting 16 weeks	2.25 (2.14, 2.35)	1.95 (1.79, 2.11)

Table 4 Mean DIB and IS-cBIC for zirconia and titanium implants at harvesting after 4 and 16 weeks of loading, respectively

	Harvesting 4 weeks	Harvesting 16 weeks	<i>P</i> value 4 to 16 weeks
Zirconia mean DIB (mm) (95% CI)	1.66 (1.56, 1.76)	2.25 (2.14, 2.35)	< 0.0001
Zirconia mean IS-cBIC (mm) (95% CI)	2.18 (2.05, 2.31)	2.48 (2.36, 2.60)	< 0.0001
<i>P</i> value zirconia histometry vs. PAs	< 0.0001	< 0.0001	
Titanium mean DIB (mm) (95% CI)	1.81 (1.65, 1.98)	1.95 (1.79, 2.11)	0.06 <i>NS</i>
Titanium mean IS-cBIC (mm) (95% CI)	2.23 (2.11, 2.36)	2.34 (2.22, 2.47)	0.27 <i>NS</i>
<i>P</i> value titanium histometry vs. PAs	< 0.0001	< 0.0001	
Mean overall DIB (mm)	1.92		
Mean overall IS-cBIC (mm)	2.31		

as 98.8% over 10 years for current implant surfaces and 89.5% over 20 years for older implant generations [3, 34]. Published data about long-term survival of commercially available zirconia implants is scarce [35]. The principal cause may be the high turnover rate typical of new medical products, as far as applicable to this relatively young material on the implant market. To the authors' knowledge, only 2 prospective clinical studies assess implant outcome of currently commercially available zirconia implants at 3 or more years of follow-up [20, 36]. Nevertheless, reports on recent—but no longer commercially available—zirconia implants demonstrate that most failures occur in the first year in function, followed by a phase with low to inexistent failure incidence [37–39]. This suggests that early to mid-term implant healing and function may be decisive for long-term outcome. In this context, preclinical *in vivo* analyses are essential (a) to establish diagnostic reference values for healthy implants, such as crestal bone remodeling over time in function, and (b) to validate accordingly non-invasive tools for early diagnosis of peri-implant health and pathology, such as PAs. Apart from the present study, only two preclinical studies using currently commercially available implants under loaded conditions are available to date [8, 40].

The present analysis demonstrated a slight reduction in DIB immediately after loading, followed by an increase between 4 and 16 weeks of function, that was more pronounced at zirconia implants. The existing literature corroborates these findings. A prospective clinical study with 71 zirconia implants found a mean marginal bone loss of 0.78 mm from implant insertion to the 1-year follow-up after the final prosthetic restoration. The peri-implant probing depth increased accordingly from 2.7 to 3.5 mm [41]. An observational clinical study demonstrated crestal bone gain of 0.66 mm between 1 and 3 years after loading, following an initial 0.44 mm loss in the first year [36]. Bone maturation at microrough titanium surfaces shows a similar pattern of BIC increase after implant placement during 4–6 weeks and subsequent decrease and stabilization in the context of bone remodeling [42]. Also, the mentioned study on loaded zirconia implants showed minimal crestal bone changes of 0.15 mm at the control titanium implant between loading and 6 months post-loading [40]. On the other hand, the authors found high variability in crestal bone loss between the 3 test zirconia implants, with a range from 0.42 mm bone gain to 0.82 mm bone loss.

**Fig. 4** PA at implant placement (a), loading (b), and after 16 weeks of loading (c) as well as histology (d) of a representative study region

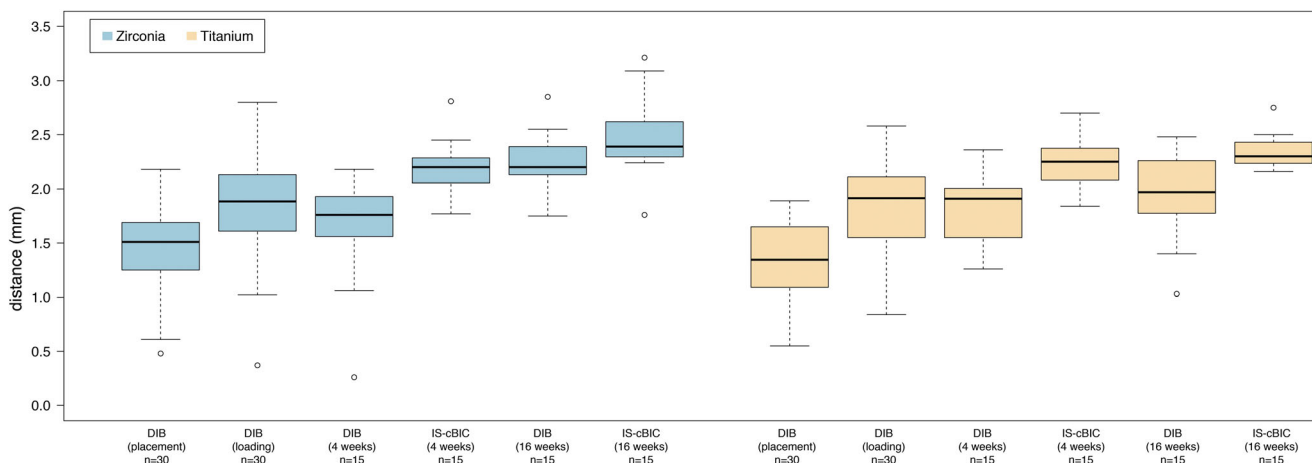


Fig. 5 Boxplots showing mean DIB for zirconia (blue) and titanium (yellow) at each time point, as well as mean IS-cBIC at 4 and 16 weeks of loading; the whiskers represent the range

Similarly, a study with unloaded implants found 0.13 mm crestal bone gain at titanium and 0.32/0.60 mm loss at two zirconia implants between 2 and 6 weeks in function [43]. Data about differences between 1- and 2-piece implant types are contradictory, with a clinical observational study showing more bone loss around 2-piece zirconia implants [44] and the mentioned animal study showing bone gain, oppositely [40].

The present investigation found a statistically significant difference between the PAs and the histometry for both materials, with radiographs yielding mean values 0.39 mm smaller than histometry on average. The discrepancy was highest for zirconia at 4 weeks (0.52 mm) and lowest for zirconia at 16 weeks (0.23 mm). A possible explanation for this difference obtained by the same implant at two time points can be searched for in the variations of peri-implant bone radiopacity over the early maturation process, which may show patterns specific to an implant material and surface. To the best of the authors' knowledge, this is the first analysis comparing PA with histometry around loaded zirconia implants. One of the earliest available animal studies with titanium implants reported that the histologic IS-cBIC was 0.85 mm more apical than measured as DIB in PAs [45]. A further analysis demonstrated high, statistically significant correlation between the two measurement methods and PA underestimating bone loss by only 0.1 mm in 73.4% of the cases [28]. When challenged with plaque accumulation and occlusal overload, respectively, DIB and IS-cBIC were on average only 0.5 and 0.1 mm apart in monkeys [46]. Moreover, this study also proved a strong, statistically significant correlation between PA and histometry. In summary, preclinical research shows (a) high reproducibility of DIB measurements in PAs through clear identifiability of crestal bone; (b) discrepancy between PA and histomorphometry of 0.1–0.85 mm, with PA generally underestimating the extent of the bone loss; and (c) sensor or film used for PA having a clear influence on the extent of the discrepancy [47].

The missing histometric analysis at the time points of implant placement and loading may be considered a major limitation of the present study. Moreover, as applicable to animal models in general, results have to be interpreted with caution due to the diverging behavior of the study subject if compared with humans. Finally, the follow-up period of maximally 16 weeks may not be sufficient to draw conclusions valid for the long-term outcome.

Conclusion

In summary, zirconia implants showed a more pronounced crestal bone loss than titanium implants between 4 and 16 weeks after loading, following initial bone gain. PAs overestimated the bone level around dental implants on average by 0.39 mm. At a closer look, underestimation of bone loss was considerable at 4 weeks for zirconia implants, whereas DIB matched histometry at 16 weeks after further tissue maturation around the same implant. Oppositely, the overestimation of crestal bone level was more linear over time at titanium implants. Bearing the discrepancy between histometry and radiography in mind, these findings further confirm PAs as non-invasive tools for early diagnosis of peri-implant health and pathology around titanium and zirconia implants.

Acknowledgments The authors gratefully acknowledge the support of Ms. Sonja Bustamante, Dr. Archie A. Jones, and Ms. Linda Torres, Department of Periodontics; and of the team at the Department of Laboratory Animals Resources, University of Texas Health Science Center at San Antonio. The accurate histologic preparation and analysis performed by Mr. David Reist, Ms. Silvia Owusu, and Ms. Margrit Rufenacht at Robert K. Schenk Laboratory of Oral Histology, School of Dental Medicine, University of Bern; and Prof. Dr. S. Milz and his team at Anatomische Anstalt Munich are highly appreciated. The authors also thank Dr. G. Raeber and Dr. M. Obrecht (Institut Straumann AG) for

providing expertise and support during the study and Ms. Jennifer Hockley for the language editing of the manuscript.

Funding information This study was funded with a research grant from the International Team for Implantology, Basel, Switzerland (ITI Grant No. 858_2012). The study materials were kindly provided by Institut Straumann AG, Basel.

Compliance with ethical standards

Conflict of interest The authors declare that they have no conflict of interest.

Ethical approval All applicable international, national, and/or institutional guidelines for the care and use of animals were followed. The study was conducted in accordance with the ethical standards of current US federal regulations. The University of Texas Health Science Center at San Antonio Institutional Animal Care and Use Committee approved animal selection, management, and study protocol prior to the start of the experiment (IACUC; ID no. 13005x).

Informed consent For this type of study, no consent other than the IACUC approval was required.

References

- Branemark PI et al (1969) Intra-osseous anchorage of dental prostheses. I. Experimental studies. *Scand J Plast Reconstr Surg* 3(2): 81–100
- Schroeder A, Stich H, Straumann F, Sutter F (1978) The accumulation of osteocementum around a dental implant under physical loading. *SSO Schweiz Monatsschr Zahnheilkd* 88(10):1051–1058
- Buser D, Janner SF, Wittneben JG, Brägger U, Ramseier CA, Salvi GE (2012) 10-year survival and success rates of 511 titanium implants with a sandblasted and acid-etched surface: a retrospective study in 303 partially edentulous patients. *Clin Implant Dent Relat Res* 14(6):839–851
- Steinemann SG (1998) Titanium—the material of choice? *Periodontol* 17:7–21
- Fage SW, Muris J, Jakobsen SS, Thyssen JP (2016) Titanium: a review on exposure, release, penetration, allergy, epidemiology, and clinical reactivity. *Contact Dermatitis* 74(6):323–345
- Petersson M, Kelk P, Belibasakis GN, Bylund D, Molin Thorén M, Johansson A (2017) Titanium ions form particles that activate and execute interleukin-1 β release from lipopolysaccharide-primed macrophages. *J Periodontol Res* 52(1):21–32
- Benic GI, Scherrer D, Sancho-Puchades M, Thoma DS, Hämmerle CH (2017) Spectrophotometric and visual evaluation of peri-implant soft tissue color. *Clin Oral Implants Res* 28(2):192–200
- Roehling S, Gahlert M, Janner S, Meng B, Woelfler H, Cochran DL (2019) Ligature-induced peri-implant bone loss around loaded zirconia and titanium implants. *Int J Oral Maxillofac Implants* 34(2): 357–365
- Roehling S, Astasov-Frauenhoffer M, Hauser-Gerspach I, Braissant O, Woelfler H, Waltimo T, Kniha H, Gahlert M (2017) In vitro biofilm formation on titanium and zirconia implant surfaces. *J Periodontol* 88(3):298–307
- Derks J, Schaller D, Håkansson J, Wennström JL, Tomasi C, Berglundh T (2016) Effectiveness of implant therapy analyzed in a Swedish population: prevalence of peri-implantitis. *J Dent Res* 95(1):43–49
- Mombelli A, Muller N, Cionca N (2012) The epidemiology of peri-implantitis. *Clin Oral Implants Res* 23(Suppl 6):67–76
- Han HJ, Kim S, Han DH (2014) Multifactorial evaluation of implant failure: a 19-year retrospective study. *Int J Oral Maxillofac Implants* 29(2):303–310
- Nascimento CD, Pita MS, Fernandes FHNC, Pedrazzi V, de Albuquerque Junior RF, Ribeiro RF (2014) Bacterial adhesion on the titanium and zirconia abutment surfaces. *Clin Oral Implants Res* 25(3):337–343
- Salihoglu U, Boynuegri D, Engin D, Duman AN, Gokalp P, Balos K (2011) Bacterial adhesion and colonization differences between zirconium oxide and titanium alloys: an in vivo human study. *Int J Oral Maxillofac Implants* 26(1):101–107
- Akagawa Y, Ichikawa Y, Nikai H, Tsuru H (1993) Interface histology of unloaded and early loaded partially stabilized zirconia endosseous implant in initial bone healing. *J Prosthet Dent* 69(6): 599–604
- Blaschke C, Volz U (2006) Soft and hard tissue response to zirconium dioxide dental implants—a clinical study in man. *Neuro Endocrinol Lett* 27(Suppl 1):69–72
- Janner SFM et al (2018) Bone response to functionally loaded, two-piece zirconia implants: a preclinical histometric study. *Clin Oral Implants Res* 29(3):277–289
- Grassi FR, Capogreco M, Consonni D, Bilardi G, Buti J, Kalemaj Z (2015) Immediate occlusal loading of one-piece zirconia implants: five-year radiographic and clinical evaluation. *Int J Oral Maxillofac Implants* 30(3):671–680
- Bormann KH, Gellrich NC, Kniha H, Schild S, Weingart D, Gahlert M (2018) A prospective clinical study to evaluate the performance of zirconium dioxide dental implants in single-tooth edentulous area: 3-year follow-up. *BMC Oral Health* 18(1):181
- Spies BC, Balmer M, Jung RE, Sailer I, Vach K, Kohal RJ (2019) All-ceramic single crowns supported by zirconia implants: 5-year results of a prospective multicenter study. *Clin Oral Implants Res* 30(5):466–475
- Pieralli S, Kohal RJ, Jung RE, Vach K, Spies BC (2017) Clinical outcomes of zirconia dental implants: a systematic review. *J Dent Res* 96(1):38–46
- Cochran DL, Obrecht M, Weber K, Dard M, Bosshardt D, Higginbottom FL, Wilson TG Jr, Jones AA (2014) Biologic width adjacent to loaded implants with machined and rough collars in the dog. *Int J Periodontics Restorative Dent* 34(6):773–779
- Ericsson I, Berglundh T, Marinello C, Liljenberg B, Lindhe J (1992) Long-standing plaque and gingivitis at implants and teeth in the dog. *Clin Oral Implants Res* 3(3):99–103
- Rocuzzo M et al (2018) Clinical outcomes of peri-implantitis treatment and supportive care: a systematic review. *Clin Oral Implants Res* 29(Suppl 16):331–350
- Buser D, Weber HP, Donath K, Fiorellini JP, Paquette DW, Williams RC (1992) Soft tissue reactions to non-submerged unloaded titanium implants in beagle dogs. *J Periodontol* 63(3): 225–235
- Weber HP, Buser D, Fiorellini JP, Williams RC (1992) Radiographic evaluation of crestal bone levels adjacent to nonsubmerged titanium implants. *Clin Oral Implants Res* 3(4): 181–188
- Cochran DL, Nummikoski PV, Higginbottom FL, Hermann JS, Maki SR, Buser D (1996) Evaluation of an endosseous titanium implant with a sandblasted and acid-etched surface in the canine mandible: radiographic results. *Clin Oral Implants Res* 7(3):240–252
- Hermann JS, Schoolfield JD, Nummikoski PV, Buser D, Schenk RK, Cochran DL (2001) Crestal bone changes around titanium implants: a methodologic study comparing linear radiographic with histometric measurements. *Int J Oral Maxillofac Implants* 16(4): 475–485

29. Sancho-Puchades M, Hammerle CH, Benic GI (2015) In vitro assessment of artifacts induced by titanium, titanium-zirconium and zirconium dioxide implants in cone-beam computed tomography. *Clin Oral Implants Res* 26(10):1222–1228
30. Smeets R, Schöllchen M, Gauer T, Aarabi G, Assaf AT, Rendenbach C, Beck-Broichsitter B, Semmusch J, Sedlacik J, Heiland M, Fiehler J, Siemonsen S (2017) Artefacts in multimodal imaging of titanium, zirconium and binary titanium-zirconium alloy dental implants: an in vitro study. *Dentomaxillofac Radiol* 46(2):20160267
31. Demirturk Kocasarac H, Ustaoglu G, Bayrak S, Katkar R, Geha H, Deahl ST 2nd, Mealey BL, Danaci M, Noujeim M (2019) Evaluation of artifacts generated by titanium, zirconium, and titanium-zirconium alloy dental implants on MRI, CT, and CBCT images: a phantom study. *Oral Surg Oral Med Oral Pathol Oral Radiol* 127(6):535–544
32. Brägger U et al (1998) Evaluation of postsurgical crestal bone levels adjacent to non-submerged dental implants. *Clin Oral Implants Res* 9(4):218–224
33. Cichetti DV (1994) Guidelines, criteria, and rules of thumb for evaluating normed and standardized assessment instruments in psychology. - *PsycNET. Psychol Assess* 6(4):284–290
34. Chappuis V, Buser R, Brägger U, Bornstein MM, Salvi GE, Buser D (2013) Long-term outcomes of dental implants with a titanium plasma-sprayed surface: a 20-year prospective case series study in partially edentulous patients. *Clin Implant Dent Relat Res* 15(6):780–790
35. Roehling S et al (2018) Performance and outcome of zirconia dental implants in clinical studies: a meta-analysis. *Clin Oral Implants Res* 29(Suppl 16):135–153
36. Kniha K, Schlegel KA, Kniha H, Modabber A, Hölzle F, Kniha K (2018) Evaluation of peri-implant bone levels and soft tissue dimensions around zirconia implants—a three-year follow-up study. *Int J Oral Maxillofac Surg* 47(4):492–498
37. Cionca N, Muller N, Mombelli A (2015) Two-piece zirconia implants supporting all-ceramic crowns: a prospective clinical study. *Clin Oral Implants Res* 26(4):413–418
38. Roehling S, Woelfler H, Hicklin S, Kniha H, Gahlert M (2016) A retrospective clinical study with regard to survival and success rates of zirconia implants up to and after 7 years of loading. *Clin Implant Dent Relat Res* 18(3):545–558
39. Jank S, Hochgatterer G (2016) Success rate of two-piece zirconia implants: a retrospective statistical analysis. *Implant Dent* 25(2):193–198
40. Thoma DS, Benic GI, Muñoz F, Kohal R, Sanz Martin I, Cantalapedra AG, Hämmerle CH, Jung RE (2015) Histological analysis of loaded zirconia and titanium dental implants: an experimental study in the dog mandible. *J Clin Periodontol* 42(10):967–975
41. Jung RE, Grohmann P, Sailer I, Steinhart YN, Fehér A, Hämmerle C, Strub JR, Kohal R (2016) Evaluation of a one-piece ceramic implant used for single-tooth replacement and three-unit fixed partial dentures: a prospective cohort clinical trial. *Clin Oral Implants Res* 27(7):751–761
42. Cochran DL, Nummikoski PV, Schoolfield JD, Jones AA, Oates TW (2009) A prospective multicenter 5-year radiographic evaluation of crestal bone levels over time in 596 dental implants placed in 192 patients. *J Periodontol* 80(5):725–733
43. Lim HC, Jung RE, Hämmerle CHF, Kim MJ, Paeng KW, Jung UW, Thoma DS (2018) Tissue integration of zirconia and titanium implants with and without buccal dehiscence defects. *J Periodontal Implant Sci* 48(3):182–192
44. Rodriguez AE, Monzavi M, Yokoyama CL, Nowzari H (2018) Zirconia dental implants: a clinical and radiographic evaluation. *J Esthet Restor Dent* 30(6):538–544
45. Caulier H, Naert I, Kalk W, Jansen JA (1997) The relationship of some histologic parameters, radiographic evaluations, and Periotest measurements of oral implants: an experimental animal study. *Int J Oral Maxillofac Implants* 12(3):380–386
46. Isidor F (1997) Clinical probing and radiographic assessment in relation to the histologic bone level at oral implants in monkeys. *Clin Oral Implants Res* 8(4):255–264
47. Stokholm R, Spin-Neto R, Nyengaard JR, Isidor F (2016) Comparison of radiographic and histological assessment of peri-implant bone around oral implants. *Clin Oral Implants Res* 27(7):782–786

Publisher's note Springer Nature remains neutral with regard to jurisdictional claims in published maps and institutional affiliations.