

Hosseini Mandana (Orcid ID: 0000-0002-8768-274X)
Jensen Simon Storgård (Orcid ID: 0000-0002-3519-4103)
Rocuzzo Andrea (Orcid ID: 0000-0002-8079-0860)

Narrow diameter implants to replace congenital missing maxillary lateral incisors: a 1-year prospective, controlled, clinical study.

Andrea ROCCUZZO^{1,2}, Jean-Claude IMBER¹, Jakob LEMPERT², Mandana HOSSEINI³, Simon Storgård JENSEN^{2,4}

¹Department of Periodontology, School of Dental Medicine, University of Bern, Bern, Switzerland;

²Department of Oral and Maxillofacial Surgery, Copenhagen University Hospital, Copenhagen, Denmark;

³Research Area Oral Rehabilitation, Section for Oral Health, Society and Technology, Institute of Odontology, Faculty of Health and Medical Sciences, University of Copenhagen, Denmark.

⁴Research Area Oral Surgery, Section for Oral Biology and Immunopathology, Institute of Odontology, Faculty of Health and Medical Sciences, University of Copenhagen, Denmark

Corresponding author:

Andrea Rocuzzo
University of Bern
School of Dental Medicine
Department of Periodontology
Freiburgstrasse 7
CH-3010 Bern, Switzerland
andrea.rocuzzo@unibe.ch

Running title: Narrow diameter implant in patients with congenitally missing lateral incisors

Acknowledgements

The authors thank Mr. Juan Luis Gómez Martínez (stHalley Statistics) for his valuable help in statistical analysis and Ms. Vibeke Nielsen (RDH) for her thorough assistance with the follow-up visits

Author contributions

A.R. and S.S.J. conceived the idea and led the writing, S.S.J performed the surgeries, J.L. performed the prosthetics, A.R., J.C.I. and M.H. collected, analyzed and interpreted the data, M.H. and J.C.I. contributed to the writing

This article has been accepted for publication and undergone full peer review but has not been through the copyediting, typesetting, pagination and proofreading process which may lead to differences between this version and the [Version of Record](#). Please cite this article as doi: [10.1111/clr.13966](https://doi.org/10.1111/clr.13966)

Funding

The study was funded by a large grant of the ITI Foundation (n 1151_2016). Implants, healing abutments, impression posts, implant analogs and standard temporary TAN abutments were provided free of charge from Straumann AG, Basel, Switzerland

Conflicts of interest

The authors declare no potential conflict of interests with respect to this study.

A.R. was the recipient of a 1-year scholarship from the Italian Society of Osseointegration (SIO) during the planning of the study. A.R. was the recipient of a 3-year scholarship from the Clinical Research Foundation (CFR) for the Promotion of Oral Health, Brienz, Switzerland. A.R. is the recipient of a 1-year scholarship from the International Team of Implantology (ITI).

Abstract

Objectives: To report the clinical, radiographic, aesthetic and patient-reported outcomes after placement of a newly developed Narrow-Diameter Implant (NDI) in patients with congenitally Missing Lateral Incisors (MLIs).

Materials and methods: Patients with MLIs with a mesio-distal distance between the canine and the central incisor of 5.9-6.3mm received a dental implant with a diameter of 2.9mm (Test), while a diameter of 3.3mm (Control) was used when the distance was 6.4-7.1mm. After healing, a cement-retained bi-layered zirconia crown was fabricated. At the 1-year follow-up (T2), implant survival rate, marginal Crestal Bone Level (CBL) changes, biological and technical complications were registered. The aesthetic outcome was assessed by using the Copenhagen Index Score, and the patient-reported outcomes were recorded using the OHIP-49 questionnaire.

Results: One-hundred patients rehabilitated with 100 dental implants Ø2.9mm (n = 50) or Ø3.3mm (n = 50) were included. One Ø3.3mm implant was lost and 7 patients dropped out of the study, yielding an implant survival rate of 99% (p = 1.000). At T2 a CBL of -0.19 ± 0.25 mm (Test) and -0.25 ± 0.31 mm (Control) was detected, with no statistically significant difference between the groups (p = 0.342). Good to excellent aesthetic scores (i.e. 1-2) were recorded in most of cases. Technical complications (i.e. loss of retention, abutment fracture, chipping of veneering ceramic) occurred once in three patients with no statistically significant difference between the groups (p > 0.05). OHIP scores did not differ significantly at follow-ups between groups (p = 0.110).

Conclusion: The use of Ø2.9mm diameter implants represents as reliable a treatment option as Ø3.3mm implants, in terms of CBL changes, biological and technical complications. Favorable aesthetics and patient-reported outcomes were recorded for both groups.

INTRODUCTION

Congenitally missing teeth, also known as tooth agenesis, is a frequent developmental dental anomaly, which may cause aesthetic and functional challenges if left untreated (Khalaf, Miskelly, Voge, & Macfarlane, 2014; Rakhshan & Rakhshan, 2016). The prevalence has been estimated to be almost 7% and the most frequently missing teeth are the mandibular second premolars (29.9%) followed by the Maxillary Lateral Incisors (MLI) (24.3%) and second premolars (13.7%) (Khalaf et al., 2014; Rakhshan & Rakhshan, 2016). The etiopathogenesis of tooth agenesis has been correlated to specific genetic syndrome (Matalova, Fleischmannova, Sharpe, & Tucker, 2008; Vastardis, 2000), even though non-syndromic hypodontia is a more frequent finding (Nieminen, Arte, Pirinen, Peltonen, & Thesleff, 1995).

Oral rehabilitation of patients with congenitally missing teeth most often requires an interdisciplinary collaboration and different well-documented treatment options frequently exist. More specifically either space closure by canine substitution or prosthetic rehabilitation represent the most frequently applied treatment modalities (Beyer, Tausche, Boening, & Harzer, 2007; Kafantaris, Tortopidis, Pissiotis, & Kafantaris, 2020; Kern, Passia, Sasse, & Yazigi, 2017; Kiliaridis, Sidira, Kirmanidou, & Michalakis, 2016; Priest, 2019).

It is widely accepted that implant-supported single unit crowns represent a reliable treatment option for the replacement of missing teeth with favorable outcomes in terms of high implant survival rate and stable peri-implant marginal bone levels (Jung, Zembic, Pjetursson, Zwahlen, & Thoma, 2012; Sailer, Muhlemann, Zwahlen, Hammerle, & Schneider, 2012; Wittneben et al., 2014). Nevertheless, in clinical scenarios with limited mesio-distal space of the edentulous area, implant placement might be challenging due to root proximity of the adjacent teeth (Richardson & Russell, 2001). Patients with congenitally missing teeth often present with reduced tooth

Accepted Article

dimensions as well as limited space in the jaws compared to patients with all permanent teeth formed (McKeown, Robinson, Elcock, al-Sharood, & Brook, 2002). To overcome these problems, and to provide patients with an implant-supported restoration with a harmonious emergence profile mimicking the contralateral tooth (M. Rocuzzo, Rocuzzo, & Ramanuskaite, 2018), Narrow Diameter Implants (NDIs) have been introduced (Zarone, Sorrentino, Vaccaro, & Russo, 2006). More specifically, following the 2018 ITI Consensus Conference, three categories of NDIs were proposed (i.e. 1: $\varnothing < 3.0$ mm (“Mini-implants”); 2: $\varnothing 3-3.25$ mm; 3: $\varnothing 3.3-3.5$ mm) (Schiegnitz & Al-Nawas, 2018). In areas of full load, concerns regarding risk of fracture of the fixtures especially after long-term of function have been raised (Galindo-Moreno et al., 2017; Ioannidis et al., 2015; Jung et al., 2018; Ma, Qi, Zhang, & Liu, 2019; Schiegnitz & Al-Nawas, 2018), even-though this risk potentially may be reduced by the introduction of new alloys such as titanium–zirconium alloy (Chiapasco, Casentini, Zaniboni, Corsi, & Anello, 2012). However, in areas of limited load, implants with a reduced diameter have shown comparable results compared to standard diameter implants. In addition, a potential advantage of using NDIs may be a reduced need for bone augmentation procedures due to the reduced diameter of the required osteotomy (A. Rocuzzo, Imber, & Jensen, 2021). So far, however, the generalizability of the reported clinical, radiographic and aesthetic outcomes of NDIs might be questionable due to the limited number of treated patients (Zarone et al., 2006) or without a control group (Lacarbonara et al., 2021).

Therefore, the aim of the present study was to test the reliability of a newly developed narrow diameter implant to replace congenitally missing lateral incisors (MLIs) in terms of implant survival rate, peri-implant marginal bone level changes, aesthetic outcome and patient-reported outcome measures (PROMS) compared to the same type of implant with a diameter of 3.3mm in a large population. The null-hypothesis (H0) was

no statistical difference in peri-implant marginal bone level changes between implants with a diameter of 2.9 mm and 3.3 mm during a 1-year follow-up period, when used to replace MLIs.

MATERIALS AND METHODS

Data reporting has been performed according to the STROBE guidelines.

Study design

The present study was designed as a prospective non-randomized controlled clinical trial with two parallel study groups, a duration period of 5 years, and was conducted at the Department of Oral & Maxillofacial Surgery, Copenhagen University Hospital, Copenhagen, Denmark. Approval to perform the study was provided by the Danish Data Protection Agency (approval number: 2012-58-0004). The investigation was conducted according to the revised principles of the Helsinki Declaration. Informed consent was obtained from each patient before beginning of the study.

Study population

From August 2016 to December 2018, patients with MLIs (i.e. 12 and/or 22) referred to the Department of Oral & Maxillofacial Surgery, Copenhagen University Hospital, Copenhagen, Denmark were consecutively enrolled and included in the present study according to the following inclusion criteria:

- age \geq 18 years
- patients with systemic health or controlled medical conditions
- arrested skeletal growth as documented by two body height measurements at least one year apart not indicating continuous growth (Jensen, 2019)

The following exclusion criteria were applied:

- contraindications to implant therapy (Hwang & Wang, 2006, 2007) including
 - o heavy smoking: >20 cigarettes/day
 - o poor oral hygiene
 - o compromised compliance
 - o periodontally compromised conditions
- patients with ML's with the canine situated in the MLI region

Study group allocation

Patients' allocation to one of the two groups of the study was determined based on the Mesio-Distal distance (MD) between the canine and the central incisor measured with a calliper. Patients with a MD of 5.9 to 6.3 mm received a dental implant with a diameter of 2.9 mm [Ø2.9 mm] (Straumann BLT implant, Roxolid®, SLActive®, Straumann AG, Basel, Switzerland), while patients presenting with MD of 6.4 mm to 7.1 mm received a dental implant with a diameter of 3.3 mm [Ø 3.3 mm] (Straumann BLT implant, Roxolid®, SLActive®).

Surgical procedure

All the surgical procedures were performed according to the manufacturers' recommendations under sterile conditions in an outpatient environment by one of the authors (S.S.J.), with more than 20 years of experience in implant dentistry. In cases of fenestration- or dehiscence-type defects, simultaneous contour augmentation was performed using Guided Bone Regeneration (GBR) by means of locally harvested autogenous bone chips applied on the exposed implant threads and subsequently covered with Demineralized Bovine Bone Mineral (DBBM) (Bio-Oss®).

Granules 0.25-1 mm, Geistlich Pharma AG, Wolhusen, Switzerland). Thereafter, the grafted area was covered by a double layer collagen membrane (Bio-Gide[®], Geistlich Pharma AG, Wolhusen, Switzerland) as described by Buser et al. (Buser et al., 2009). In cases of facial bone wall thickness after implant osteotomy of <1.7 mm, GBR was performed using DBBM alone covered with a double layer collagen membrane on the buccal aspect to protect against additional resorption and to support the soft tissue contour. Finally, a conical healing abutment (Straumann SC Healing Abutment narrow and standard connections, 2) was mounted, and the flap was repositioned and sutured to allow a tension-free healing. Details of the surgical procedures have been previously reported (A. Rocuzzo et al., 2021).

Prosthetic procedure

All the prosthetic procedures followed the manufacturer's instructions for the type of reconstruction in question and were performed by one experienced prosthodontist (J.L.) with more than 10 years of experience in implant prosthodontics.

All restorations were fabricated by the same Dental Laboratory (CC Dent, Copenhagen, Denmark) by the same experienced dental technician, using identical materials and technical procedure. After a healing period of 3 months (Type 4-C placement and loading according to Gallucci and co-workers (Gallucci, Hamilton, Zhou, Buser, & Chen, 2018)), impressions were taken at fixture level using a polyether material (Impregum; 3M Espe, Seefeld, Germany) to fabricate provisional screw-retained, laboratory cemented PolyMethylMethAcrylate (PMMA) single-unit crowns on temporary abutments (Straumann NC and SC, 1-3mm gingival height), which were mounted and adjusted to slight or no occlusion.

After an additional period of 3 months, a second impression of the mucosal tissue was taken and a new mucosa model, on the original master model, was made. The patient

Accepted Article

was referred to the laboratory and color measurement was performed. A Straumann CARES Titanium abutment was CAD/CAM designed and manufactured and a feldspathic-ceramic-veneered-zirconia crown was fabricated. Final adjustment of color was performed by the laboratory. The crown was returned to the prosthodontist. The provisional crown was removed, abutment was mounted and torqued according to the manufacturer's instructions. The screw channel was blocked with sterilized PTFE-tape and cemented with Zinc-phosphate cement either Hoffmann's Phosphate cement, Colour 03 (Hoffmann Dental Manufactur GMBH, Berlin, Germany) or Detray Zinc-phosphate cement (Dentsply Detrey GmbH, Germany). Excess cement was carefully removed with a periodontal probe and dental floss (Oral B, Superfloss, Procter & Gamble UK, Waybridge, Surrey, UK) and complete removal was thereafter checked radiographically. Finally, impression in Alginot (Kerr Corporation, USA) was made and a 1.5 mm thermoplastic protection night-guard (Scheu Dental GmbH, Germany) was fabricated for the upper jaw. Patients were finally given careful instructions on proper oral hygiene. This appointment was considered the baseline examination (T1).

Supportive periodontal/peri-implant program and follow-up examination

At the completion of the rehabilitation phase (T1), patients were referred to their private dental practitioners for individual maintenance programs. Patients were invited for a follow-up examination 1-year after crown delivery which was considered the 1-year examination (T2).

Outcomes measures

For the record and analysis of the investigated outcomes three different time points were defined:

- T0: time of the implant placement. Pre- and intra-operative clinical measurements, radiographic Crestal Bone Level (CBL)
- T1: delivery of the final reconstruction (i.e. baseline). Radiographic Crestal Bone Level (CBL), aesthetic assessment of the Copenhagen Index Score.
- T2: follow-up examination (i.e. 1-year after baseline). Assessment of implant survival rate, radiographic Crestal Bone Level (CBL), aesthetic assessment

Oral Health Impact Profile-49 (OHIP-49) questionnaires were filled in just before initiation of the prosthetic phase at impression taking for the temporary implant-supported Fixed Dental Prosthesis (FDP) approximately 3 months after T0 and at T2.

Implant and reconstruction survival

Implant survival rate was calculated at patient level, which was identical to implant level since only one implant was included per patient, and was defined as the presence of the installed implant in the oral cavity. Reconstruction survival rate was defined as the presence of the implant-supported single-unit crown on the implant.

Biological and technical complications

At the 1-year follow-up (T2) clinical examination, performed by an experienced dental hygienist under supervision of the senior author (S.S.J.), the clinical examination included the assessment at each implant site of the following biological parameters:

- Peri-implant probing depth in mm at six sites per implant
- Plaque Score: presence or absence at implant site (0/1)
- Exudation or suppuration after probing (0/1)

- Presence of fistula
- Pain
- Necrosis of the neighboring teeth

The following technical complications were recorded:

- Loosening or fracture of the abutment
- Loss of retention of the reconstruction (i.e. decementation of the reconstruction)
- Fracture or chipping of the veneering ceramic

Radiographic assessment

Peri-apical radiographs were taken after implant placement (T0), after crown delivery (T1) and at the 1-year follow-up examinations (T2). Digital non-standardized and non-individualized intraoral radiographs were obtained using the paralleling technique. Images were then imported in a dedicated software (Zen pro, Carl Zeiss AG, Oberkochen, Germany). The known implant lengths (i.e. 10 or 12 mm) were used to calibrate the images (Figure 2). Crestal Bone Levels (CBL) were assessed on both the mesial and distal peri-implant surface as the linear distance between the implant shoulder and the first bone to implant contact. Changes in CBL were calculated by subtracting the T1 value from the T2 value. Therefore, all positive values indicated bone gain, while bone loss was defined by negative values. All radiographic measurements were taken independently and in duplicate by two of the authors (A.R.; J-C.I.) not involved in any part of the treatment and follow-up examinations.

Aesthetic assessment (Copenhagen Index Score and supplementary implant-related aesthetic parameters)

The aesthetic assessment was performed from frontal and semi-axial clinical photographs of the restorations, including the adjacent teeth and marginal peri-implant

mucosa taken at T1 and T2 (A. Rocuzzo, Jensen, Worsaae, & Gotfredsen, 2020). To assess the aesthetic outcomes, the Copenhagen Index Score (CPHI) was used as described by Dueled and co-workers (Dueled, Gotfredsen, Trab Damsgaard, & Hede, 2009) and Hosseini & Gotfredsen (Hosseini & Gotfredsen, 2012) with all the evaluated parameters scored from 1 (i.e. optimal) to 4 (i.e. not-sufficient) (Table 4).

More specifically, the following parameters were assessed:

- Symmetry/harmony: assessment according to facial midline, tooth axis, contralateral tooth and smile line. Score 1: excellent; score 2: suboptimal but satisfactory; score 3: moderate; score 4: poor symmetry and harmony
- Crown morphology: assessment in relation to anatomy, surface texture, contour, prominence, contact points, crown length and crown width in relation to neighboring teeth. Score 1: excellent; score 2: satisfactory, but suboptimal in one or two of the sub-parameters; score 3: moderate with suboptimal for several sub-parameters; score 4: was poor concerning most of the sub-parameters
- Crown color: assessment according to the hue value, chroma and translucency of the implant-supported crown compared with neighboring teeth. Score 1 excellent color and not easy to distinguish from the natural, neighboring teeth; score 2 was satisfactory, almost optimal but the reconstruction differed from the natural, neighboring teeth; score 3 was moderate, suboptimal color, and score 4 was poor color match.
- Soft tissue score: Score 1: no discoloration, score 2: light greyish discoloration, score 3: distinguishable greyish discoloration, score 4: metal or abutment visible.
- Papilla index: Score 1: papilla filling the entire proximal space; score 2: papilla filling at least half of the entire proximal space; score 3: papilla filling less than half of the proximal space, score 4: no papilla.

- Level of the margin: assessment of the apically or incisal position of the buccal marginal peri-implant mucosa in the middle of the implant crown compared to the contralateral tooth or the neighboring teeth. Score 1: match; score 2: slight mismatch; score 3: moderate mismatch; score 4: mismatch.
- Soft tissue texture: assessment related to the smoother or rougher surface texture of the buccal peri-implant mucosa compared to natural gingiva at the contralateral tooth or the neighboring teeth. Score 1: match; score 2: slight mismatch; score 3: moderate mismatch; score 4: distinct mismatch.
- Soft tissue curvature: assessment according to the over-contoured or under-contoured buccal marginal peri-implant mucosa compared to natural gingiva at the contralateral tooth or the neighboring teeth. Score 1: match; score 2: slight mismatch; score 3: moderate mismatch; score 4: distinct mismatch.
- Alveolar process deficiency: assessment related to the concavity or convexity of the buccal peri-implant mucosa compared to the natural contour of the buccal gingiva at the contralateral tooth or the neighboring teeth. Score 1: match; score 2: slight mismatch; score 3: moderate mismatch; score 4: distinct mismatch.
- Marginal adaptation score: radiological assessment of fit or any gap between the implant crown and the abutment mesially and/or distally. Score 1: excellent fit; score 2: distinguishable misfit; score 3: distinct misfit; score 4: unacceptable misfit.
- Cement excess: radiographic presence (score 1) or absence (score 0) of cement in relation to the implant crowns

A periodontist (A.R.) and a prosthodontist (M.H.) not involved in any part of the treatments assessed the aesthetic parameters. In cases of disagreement, the senior author (S.S.J.) was asked to provide his assessment and consensus was reached

following discussion. All assessments were blinded regarding the implant diameters and were recorded as frequencies.

Patient-reported outcomes assessment

The impact on oral health-related quality of life was evaluated using a validated Danish version of the OHIP-49 questionnaire before prosthetic treatment (i.e. before impression taking for the temporary crown) and at the 1-year follow-up examination. Each patient was asked to score each question with a Likert response scale from 0 (never experienced problem) to 4 (problem experienced very often). The summary of questions 3, 4, 20, 22, 31 and 38 was used to describe the patient-reported “aesthetic outcome” (Dueled et al., 2009), while the “masticatory function” was expressed by the summary scores of questions 1, 28, 29 and 32 (Goshima et al., 2010). The overall oral health-related impact on quality of life was described by the sum of scores from all 49 OHIP questions before prosthetic treatment, and one year after loading.

Statistical Analysis

In cases with bilateral MLIs, where implants with identical diameters were placed, only one implant was randomly selected for the statistical analysis (www.randomization.com).

Sample size calculation

Sample size calculation was performed on the secondary outcome parameter: peri-implant crestal bone resorption according to Hosseini et al., 2013 (Hosseini, Worsaae, Schiodt, & Gotfredsen, 2013). More in detail, a mean crestal bone loss of 0.6 mm in the test group and 0.2 mm in the control group were considered significant. Therefore, in order to detect a difference of 0.4 mm and a standard deviation of 0.6, 49 patients

per group were needed with an alpha (type I error) = 0.05 and a pf power= 0.9. Using an independent sample t-Test a group size of N= 49 was calculated. Patients number per group was rounded to 50.

Data analysis

Each patient contributed with one dental implant only and was, therefore, considered as the statistical unit. Descriptive analysis was performed providing absolute and relative frequencies for categorical variables and mean, standard deviation, for continuous variables. Normal distribution of the quantitative measures was checked by Kolmogorov-Smirnov test. Two-sample t-test was used to compare mean CBL between both implant groups. The calculated inter-examiner agreement with Dahlberg's d test was in the range 0.09-0.14 mm and the Intra-Class correlation Coefficient (ICC) was in the range 0.95-0.98 providing a very high level of reproducibility of the performed measurements.

Chi² independence, Kendall's Tau-b and Fisher's exact test were used to assess the association between categorical/ordinal aesthetic variables and group. Similar tests were used to compare collected parameters (i.e. width of the alveolar process (WAP), Width of the Alveolar Ridge (WAR), Thickness of the Facial Bone (TFB) after osteotomy) and need of bone regeneration between groups. Paired t-test was used for intra-group comparisons of the OHIP scores over time. All the tests were two-tailed and the level of significance was set at 5%. The statistical analysis was performed with a commercially available dedicated software (SPSS 15.0, Chicago, IL., USA).

RESULTS

Study sample characteristics

The investigated population included 100 patients rehabilitated with 100 dental implants \varnothing 2.9 mm (n = 50) or \varnothing 3.3 mm (n = 50). All 100 patients underwent pre-operative orthodontic treatment to allow implant placement. At the time of implant placement, the mean age was 21.5 ± 2.6 years (range: 18–31) and did not statistically significant differ between groups ($p = .258$). The gender distribution (male:female) in the whole sample was 1:1.44 and in the two groups \varnothing 2.9 mm: 1:1.94 versus. \varnothing 3.3 mm: 1:1.08 ($p = .155$). During the implant placement procedure, 34 implants with \varnothing 3.3 mm and 22 with a \varnothing 2.9 mm needed a bone augmentation procedure ($p = .017$). No soft tissue augmentation procedures were performed simultaneous with implant placement. Additional data on the population have been reported in Rocuzzo et al. 2021. At the 1-year follow-up examination, a total of 7 drop-out patients (\varnothing 2.9 mm (n = 3); \varnothing 3.3 mm (n = 4)) were recorded.

Details of the patients' characteristic and reasons for drop-outs are listed in Table 1 and 2. The overall study flow is presented in Figure 1.

Biological outcome parameters

Of the 93 patients available for follow-up, one patient with a \varnothing 3.3 mm experienced implant loss before loading (i.e. early implant failure) leading to an implant survival rate of 100% in the \varnothing 2.9 mm group and 98% in the \varnothing 3.3 mm group with no statistically significant difference between the two groups ($p = 1.000$; 95% C I: 94.6-99.9%).

With respect to mean CBL changes no statistically significant differences were detected at any time points (T1-T0; T2-T0; T2-T1) within the 2 groups: more specifically, in the first year after loading (i.e. T2-T1) a CBL of -0.19 ± 0.25 mm in the \varnothing 2.9 mm and -0.25 ± 0.31 mm \varnothing 3.3 mm was detected, with no statistically significant

Accepted Article

difference between the groups ($p = 0.342$). Details of CBL changes over time are provided in Figure 3.

Mean Peri-Implant Probing Depth (PPD) value was 2.55 ± 0.41 mm in the $\text{Ø}2.9$ mm group and 2.50 ± 0.45 mm in $\text{Ø}3.3$ mm group, with no statistically significant difference between groups ($p = 0.576$).

Plaque scores did not statistically significant differ between the 2 groups: 15% in the $\text{Ø}2.9$ mm group and 12% in the in $\text{Ø}3.3$ mm group ($p = 0.631$).

Presence of a buccal fistula was recorded in 4 cases at the 1-year follow-up visit (2 per group) (Figure 4a), while suppuration after probing was detected around 2 implants (1x per group). None of the neighboring teeth displayed radiographic nor clinical signs of endodontic complications.

Technical outcome parameters

One event of a loosening abutment screw was detected in the $\text{Ø}3.3$ mm group, while loss of retention of the reconstruction occurred twice in the $\text{Ø}2.9$ mm and once in the $\text{Ø}3.3$ mm group. None of the restorations had to be remade due to unacceptable marginal adaptation (i.e. Score 4). Finally, radiographic evidence of cement excesses was observed twice at the 1-year examination (1x $\text{Ø}2.9$ mm; 1x $\text{Ø}3.3$ mm group).

The biological and technical complications are reported in Table 3a-b.

Aesthetic outcome parameters

The assessment of the aesthetic presentation of the implant-supported single-crowns showed good to optimal results (i.e. scores 1 and 2) at T2, irrespective of the implant diameter, in the majority of the cases (i.e. variables: Symmetry; Soft tissue color; Soft tissue curvature; Alveolar process deficiency) ($p > 0.05$). Nevertheless, peri-implant soft tissue score 3 (i.e. presence of discoloration) was detected in 13% of the $\text{Ø}2.9$ mm

and 2.4% in the Ø3.3 mm ($p = 0.747$). With respect to papilla fill, no statistically significant differences were identified between the groups at T2 in terms of mesial ($p=0.420$) and distal ($p = 0.073$) papilla index score.

Details of the aesthetic outcomes are listed in Table 4.

Patient-reported outcome parameters

Table 5 summarizes the patient-reported aesthetic outcome, masticatory function and overall oral health-related impact on quality of life in all patients from before delivery of the final reconstruction until the 1-year control. During the observation period, a decrease in all the scores with respect to the both the aesthetic and masticatory functions analysis were detected indicating subjective improvement without a statistically significant difference between the groups ($p > 0.05$). Moreover, the summary scores of the 49 OHIP questions decreased through the study period indicating an overall improvement in oral health-related impact on quality of life with no statistically significant difference between the two groups ($p > 0.05$).

DISCUSSION

The present study could not demonstrate any statistical differences in terms of implant survival, crestal bone loss, aesthetic outcome or patient-reported outcome measures between narrow diameter implants with a diameter of 2.9 mm or 3.3mm for replacement of MLIs after one year of loading. The null hypothesis of no difference in peri-implant marginal bone level changes after one year of loading could therefore not be rejected.

With respect to the outcome implant survival, high percentages within both groups, were recorded: our results are in accordance with those reported by Schiegnitz & Al-Nawas (Schiegnitz & Al-Nawas, 2018) who have calculated an implant survival rate of $94.7 \pm 5\%$ for implants with a diameter < 3.0 mm and $97.7 \pm 2.3\%$ with a diameter of 3.3-3.5 mm for single unit-gap tooth replacement, respectively.

Historically, reduced peri-implant crestal bone resorption has been reported around Standard Diameter Implants (SDIs) compared to NDIs, which has mainly been ascribed to a better distribution of occlusal forces around a wider implant (Qian, Todo, Matsushita, & Koyano, 2009). During recent years, several clinical studies have reported good clinical outcomes and limited radiographic CBL changes (<1 mm) for NDIs short-term (Degidi, Nardi, & Piattelli, 2009; Maiorana et al., 2015; Reddy, O'Neal, Haigh, Aponte-Wesson, & Geurs, 2008) as well as long-term (Branzén, Eliasson, Arnrup, & Bazargani, 2015; Galindo-Moreno et al., 2017). In accordance with previous studies, the present study identified the major part of crestal remodeling to take place between implant placement and prosthetic loading. This process might be explained as the physiologic bone remodeling following sub-crestal implant placement with the concomitant establishment of the peri-implant soft-tissue seal (Berglundh, Abrahamsson, Welander, Lang, & Lindhe, 2007; Cardaropoli, Lekholm, & Wennström,

2006). After prosthetic loading only minimal crestal bone loss was observed which is compatible with generalized healthy peri-implant conditions as expected in a young healthy population (Santing, Raghoobar, Vissink, den Hartog, & Meijer, 2013).

With respect to the recorded biological complications, two implants per group developed a buccal fistula without suppuration not associated with an increasing peri-implant probing depth nor in the CBL changes (Figure 4a). Similar findings have previously been correlated to the presence of subgingival remnants of cement (Bonde, Stokholm, Isidor, & Schou, 2010) or suboptimal marginal adaptation of the crowns (Gottfredsen, 2004). However, no such problems could be identified around the four implants, and it was decided to observe the conditions at the following control visits.

The use of NDIs has been correlated to an increased risk for technical complications due to their weaker structure (Shi et al., 2018). Nevertheless, in the present study, only minor complications (i.e. 1x loosening of the abutment screw and chipping of veneering ceramic (Figure 4b)) were recorded and could be handled without negatively affecting the survival of the restoration. More specifically, it should be underlined that at the time of crown delivery, a careful check of the occlusal contacts and lateral guidance has been performed to minimize the risks of premature contacts which could have had a detrimental effect of the implant-supported restoration. One of the most frequently reported technical complications is decementation of the reconstruction (Woelber, Ratka-Krueger, Vach, & Frisch, 2016). In the investigated cohort, two events in the Ø 2.9 mm group and one in the Ø 3.3 mm group were recorded. These results are consistent with those reported in the literature (King et al., 2016; Lee et al., 2013).

Aesthetics is considered as one of the most important aspect of oral rehabilitation in the maxillary anterior region. In the present study, especially due to the young age of the included patients, every effort was made to maximize the aesthetic outcomes (Figure 5a-b) as demonstrated by the high percentage of good to optimal crown

morphology and colors. Nevertheless, it must be underlined that differences at the time of the crown delivery between the groups with respect to the crown morphology and crown color were detected (<0.001). These differences might be speculated to be related primary to the prosthetic manufacturing phase than to the implant diameter. In addition, due to the high number of included patients, slight differences in the aesthetic assessment (i.e. Score 1 vs. 2) can be easier detected, as within the present cohort.

When focusing on the peri-implant soft tissue conditions, it has to be underlined that at the 1-year follow-up, a consistent number of patients exhibited a soft tissue color mismatch (i.e. greyness or redness). One possible explanation of this color mismatch might be the use of a Titanium abutments. Zirconia abutments may be preferable over metal abutments to reduce the risk of peri-implant mucosal discoloration (Bidra & Rungruanganunt, 2013; Linkevicius & Vaitelis, 2015; Totou, Naka, Mehta, & Banerji, 2021). However, other studies indicated no differences in the peri-implant mucosa discoloration between the zirconia and metal abutments (Hosseini, Worsaae, Schiødt, & Gotfredsen, 2011; Hosseini, Worsaae, Schiødt, & Gotfredsen, 2013). Moreover, since zirconia abutments are not available for the Ø2.9mm implants, titanium fabricated abutments had to be used in order to have only one type of abutment with no difference between test and control groups.

One of the interesting findings from the present study is that more than 60% of cases scored as “optimal” (i.e. Score 1) with respect to the alveolar process deficiency evaluation have received a bone augmentation procedure either with DBBM alone or DBBM in combination with autogenous bone, providing an indirect evidence of the need for grafting procedure at the time of implant placement to allow an optimal peri-implant soft tissue architecture (Table 6). On the other hand, it has to be underlined that a minimum of 1.7mm of facial bone wall was not able to avoid the development of alveolar process deficiency as demonstrated by the 40% of cases at T2 that scored 2

(i.e. slight deficiency). One possible explanation is that, at the time of implant placement no soft tissue grafting procedures were performed in order to limit the intra-operative morbidity since most of the implants already required a bone regenerative procedure. Nevertheless, during recent years soft-tissue grafting procedures in the aesthetic zone have shown promising results and gained increased popularity and have become standard of care (Thoma et al., 2021).

Since their introduction in 2008 (Lang et al. 2008), PROMs have received increasing focus for the evaluation of implant-supported rehabilitations (Duong et al., 2022). The results from the present study have shown a general improvement in patient-reported outcomes irrespective of the implant diameter, which may be explained by the overall high quality of the provided treatments. Indeed, it is well known that most of the patients undergoing implant placement for the replacement MLIs have reported lower baseline-scores as consequence of dissatisfaction with the temporary removable restorations and the long-term orthodontic pre-treatment (Gotfredsen, 2012). With respect to the aesthetic and masticatory function scores, our results are consistent with previous publications (Feine et al., 2018; Gotfredsen, 2012; Pjetursson, Karoussis, Bürgin, Brägger, & Lang, 2005).

This study presents some limitations: firstly, despite the large sample size, it has to be pointed out that the selection of implant diameter should be based on the accurate analysis of several anatomical (i.e. available amount of bone) and prosthetic factors (i.e. expected functional load and on the emergence profile) and not only depending on mesio-distal gap dimension. On this point, it has to be mentioned that the functional load in the region of the MLI is in considered low. However, for aesthetic reasons, it was not considered ethical to place a Ø 2.9 mm implant when the mesio-distal space allowed placement of a Ø 3.3 mm implant. Indeed, narrow diameter implants placed in wide tooth gaps need to be placed vertically deeper to allow a harmonious emergence

Accepted Article

profile which may be accompanied by a risk of increased peri-implant pocket depth. Consequently, the present study could not be planned as a randomized controlled study and direct comparison between the two groups should therefore be done with caution. Moreover, even-though it is widely accepted that implant-supported single-crowns in the aesthetic area should be screw-retained (Wittneben, Joda, Weber, & Brägger, 2017), all the reconstructions of the present studies were cemented. The reason for this was that at the time of the study initiation (i.e. 2016) original components to support a screw-retained implant-supported single-crowns were not available for the Ø 2.9 mm implants. In order to have only one type of crown retention without differences between test and control, all the definitive crowns were cemented. Furthermore, it has to be mentioned that this study has been designed with the focus on the hard-tissue conditions and that of a precise assessment of the peri-implant soft-tissue dehiscence is lacking. Finally, due to the limited follow-up period (i.e. 12 months), the presented clinical and radiographic outcomes should be interpreted with caution and additional long-term studies (i.e. 3- and 5-years) including the assessment of mechanical stability, infraposition, the presence of missing contact points and peri-implant soft-tissue margin changes will provide relevant information.

In conclusion, within the limitations of the present short-term study, the use of an implant with a diameter of 2.9 and 3.3 mm showed equivalent performance in terms of survival rate, CBL changes, aesthetic and patients-reported outcomes. Consequently, clinicians should consider the use of such NDIs in case of replacement of maxillary lateral incisors especially when limited mesio-distal space otherwise would challenge the possibility implant treatment.

References

- Berglundh, T., Abrahamsson, I., Welander, M., Lang, N. P., & Lindhe, J. (2007). Morphogenesis of the peri-implant mucosa: an experimental study in dogs. *Clin Oral Implants Res*, 18(1), 1-8. doi:10.1111/j.1600-0501.2006.01380.x
- Beyer, A., Tausche, E., Boening, K., & Harzer, W. (2007). Orthodontic space opening in patients with congenitally missing lateral incisors. *Angle Orthod*, 77(3), 404-409. doi:10.2319/0003-3219(2007)077[0404:Osoipw]2.0.Co;2
- Bidra, A. S., & Rungruanunt, P. (2013). Clinical outcomes of implant abutments in the anterior region: a systematic review. *J Esthet Restor Dent*, 25(3), 159-176. doi:10.1111/jerd.12031
- Bonde, M. J., Stokholm, R., Isidor, F., & Schou, S. (2010). Outcome of implant-supported single-tooth replacements performed by dental students. A 10-year clinical and radiographic retrospective study. *Eur J Oral Implantol*, 3(1), 37-46.
- Branzén, M., Eliasson, A., Arnrup, K., & Bazargani, F. (2015). Implant-Supported Single Crowns Replacing Congenitally Missing Maxillary Lateral Incisors: A 5-Year Follow-Up. *Clin Implant Dent Relat Res*, 17(6), 1134-1140. doi:10.1111/cid.12233
- Buser, D., Halbritter, S., Hart, C., Bornstein, M. M., Grutter, L., Chappuis, V., & Belser, U. C. (2009). Early implant placement with simultaneous guided bone regeneration following single-tooth extraction in the esthetic zone: 12-month results of a prospective study with 20 consecutive patients. *J Periodontol*, 80(1), 152-162. doi:10.1902/jop.2009.080360
- Cardaropoli, G., Lekholm, U., & Wennström, J. L. (2006). Tissue alterations at implant-supported single-tooth replacements: a 1-year prospective clinical study. *Clin Oral Implants Res*, 17(2), 165-171. doi:10.1111/j.1600-0501.2005.01210.x
- Chiapasco, M., Casentini, P., Zaniboni, M., Corsi, E., & Anello, T. (2012). Titanium-zirconium alloy narrow-diameter implants (Straumann Roxolid®) for the rehabilitation of horizontally deficient edentulous ridges: prospective study on 18 consecutive patients. *Clin Oral Implants Res*, 23(10), 1136-1141. doi:10.1111/j.1600-0501.2011.02296.x
- Degidi, M., Nardi, D., & Piattelli, A. (2009). Immediate restoration of small-diameter implants in cases of partial posterior edentulism: a 4-year case series. *J Periodontol*, 80(6), 1006-1012. doi:10.1902/jop.2009.080649
- Dueled, E., Gotfredsen, K., Trab Damsgaard, M., & Hede, B. (2009). Professional and patient-based evaluation of oral rehabilitation in patients with tooth agenesis. *Clin Oral Implants Res*, 20(7), 729-736. doi:10.1111/j.1600-0501.2008.01698.x
- Duong, H. Y., Rocuzzo, A., Stähli, A., Salvi, G. E., Lang, N. P., & Sculean, A. (2022). Oral health-related quality of life of patients rehabilitated with fixed and removable implant-supported dental prostheses. *Periodontol 2000*. doi:10.1111/prd.12419
- Feine, J., Abou-Ayash, S., Al Mardini, M., de Santana, R. B., Bjelke-Holtermann, T., Bornstein, M. M., . . . Zubiria, J. P. V. (2018). Group 3 ITI Consensus Report: Patient-reported outcome measures associated with implant dentistry. *Clin Oral Implants Res*, 29 Suppl 16, 270-275. doi:10.1111/clr.13299
- Galindo-Moreno, P., Nilsson, P., King, P., Worsaae, N., Schramm, A., Padiá-Molina, M., & Maiorana, C. (2017). Clinical and radiographic evaluation of early loaded narrow-diameter implants: 5-year follow-up of a multicenter prospective clinical study. *Clin Oral Implants Res*, 28(12), 1584-1591. doi:10.1111/clr.13029
- Gallucci, G. O., Hamilton, A., Zhou, W., Buser, D., & Chen, S. (2018). Implant placement and loading protocols in partially edentulous patients: A systematic review. *Clin Oral Implants Res*, 29(S16), 106-134. doi:<https://doi.org/10.1111/clr.13276>

- Goshima, K., Lexner, M. O., Thomsen, C. E., Miura, H., Gotfredsen, K., & Bakke, M. (2010). Functional aspects of treatment with implant-supported single crowns: a quality control study in subjects with tooth agenesis. *Clin Oral Implants Res*, *21*(1), 108-114. doi:10.1111/j.1600-0501.2009.01809.x
- Gotfredsen, K. (2004). A 5-year prospective study of single-tooth replacements supported by the Astra Tech implant: a pilot study. *Clin Implant Dent Relat Res*, *6*(1), 1-8. doi:10.1111/j.1708-8208.2004.tb00021.x
- Gotfredsen, K. (2012). A 10-year prospective study of single tooth implants placed in the anterior maxilla. *Clin Implant Dent Relat Res*, *14*(1), 80-87. doi:10.1111/j.1708-8208.2009.00231.x
- Hosseini, M., & Gotfredsen, K. (2012). A feasible, aesthetic quality evaluation of implant-supported single crowns: an analysis of validity and reliability. *Clin Oral Implants Res*, *23*(4), 453-458. doi:10.1111/j.1600-0501.2011.02162.x
- Hosseini, M., Worsaae, N., Schiodt, M., & Gotfredsen, K. (2011). A 1-year randomised controlled trial comparing zirconia versus metal-ceramic implant supported single-tooth restorations. *Eur J Oral Implantol*, *4*(4), 347-361.
- Hosseini, M., Worsaae, N., Schiødt, M., & Gotfredsen, K. (2013). A 3-year prospective study of implant-supported, single-tooth restorations of all-ceramic and metal-ceramic materials in patients with tooth agenesis. *Clin Oral Implants Res*, *24*(10), 1078-1087. doi:10.1111/j.1600-0501.2012.02514.x
- Hwang, D., & Wang, H. L. (2006). Medical contraindications to implant therapy: part I: absolute contraindications. *Implant Dent*, *15*(4), 353-360. doi:10.1097/01.id.0000247855.75691.03
- Hwang, D., & Wang, H. L. (2007). Medical contraindications to implant therapy: Part II: Relative contraindications. *Implant Dent*, *16*(1), 13-23. doi:10.1097/ID.0b013e31803276c8
- Ioannidis, A., Gallucci, G. O., Jung, R. E., Borzangy, S., Hammerle, C. H., & Benic, G. I. (2015). Titanium-zirconium narrow-diameter versus titanium regular-diameter implants for anterior and premolar single crowns: 3-year results of a randomized controlled clinical study. *J Clin Periodontol*, *42*(11), 1060-1070. doi:10.1111/jcpe.12468
- Jensen, S. S. (2019). Timing of Implant Placement after Traumatic Dental Injury. *J Endod*, *45*(12s), S52-s56. doi:10.1016/j.joen.2019.05.013
- Jung, R. E., Al-Nawas, B., Araujo, M., Avila-Ortiz, G., Barter, S., Brodala, N., . . . Windisch, P. (2018). Group 1 ITI Consensus Report: The influence of implant length and design and medications on clinical and patient-reported outcomes. *Clin Oral Implants Res*, *29 Suppl 16*, 69-77. doi:10.1111/clr.13342
- Jung, R. E., Zembic, A., Pjetursson, B. E., Zwahlen, M., & Thoma, D. S. (2012). Systematic review of the survival rate and the incidence of biological, technical, and aesthetic complications of single crowns on implants reported in longitudinal studies with a mean follow-up of 5 years. *Clin Oral Implants Res*, *23 Suppl 6*, 2-21. doi:10.1111/j.1600-0501.2012.02547.x
- Kafantaris, S. N., Tortopidis, D., Pissiotis, A. L., & Kafantaris, N. M. (2020). Factors Affecting Decision-Making For Congenitally Missing Permanent Maxillary Lateral Incisors: A Retrospective Study. *Eur J Prosthodont Restor Dent*, *28*(1), 43-52. doi:10.1922/EJPRD_1959Kafantaris10
- Kern, M., Passia, N., Sasse, M., & Yazigi, C. (2017). Ten-year outcome of zirconia ceramic cantilever resin-bonded fixed dental prostheses and the influence of the reasons for missing incisors. *J Dent*, *65*, 51-55. doi:10.1016/j.jdent.2017.07.003
- Khalaf, K., Miskelly, J., Voge, E., & Macfarlane, T. V. (2014). Prevalence of hypodontia and associated factors: a systematic review and meta-analysis. *J Orthod*, *41*(4), 299-316. doi:10.1179/1465313314y.0000000116

- Kiliaridis, S., Sidira, M., Kirmanidou, Y., & Michalakis, K. (2016). Treatment options for congenitally missing lateral incisors. *Eur J Oral Implantol*, *9 Suppl 1*, S5-24.
- King, P., Maiorana, C., Luthardt, R. G., Sondell, K., Øland, J., Galindo-Moreno, P., & Nilsson, P. (2016). Clinical and Radiographic Evaluation of a Small-Diameter Dental Implant Used for the Restoration of Patients with Permanent Tooth Agenesis (Hypodontia) in the Maxillary Lateral Incisor and Mandibular Incisor Regions: A 36-Month Follow-Up. *Int J Prosthodont*, *29*(2), 147-153. doi:10.11607/ijp.4444
- Lacarbonara, M., Cazzolla, A. P., Lacarbonara, V., Lo Muzio, L., Ciavarella, D., Testa, N. F., ... Capogreco, M. (2021). Prosthetic rehabilitation of maxillary lateral incisors agenesis using dental mini-implants: a multicenter 10-year follow-up. *Clin Oral Investig*. doi:10.1007/s00784-021-04176-0
- Lee, J. S., Kim, H. M., Kim, C. S., Choi, S. H., Chai, J. K., & Jung, U. W. (2013). Long-term retrospective study of narrow implants for fixed dental prostheses. *Clin Oral Implants Res*, *24*(8), 847-852. doi:10.1111/j.1600-0501.2012.02472.x
- Linkevicius, T., & Vaitelis, J. (2015). The effect of zirconia or titanium as abutment material on soft peri-implant tissues: a systematic review and meta-analysis. *Clin Oral Implants Res*, *26 Suppl 11*, 139-147. doi:10.1111/clr.12631
- Ma, M., Qi, M., Zhang, D., & Liu, H. (2019). The Clinical Performance of Narrow Diameter Implants Versus Regular Diameter Implants: A Meta-Analysis. *J Oral Implantol*, *45*(6), 503-508. doi:10.1563/aaid-joi-D-19-00025
- Maiorana, C., King, P., Quaas, S., Sondell, K., Worsaae, N., & Galindo-Moreno, P. (2015). Clinical and radiographic evaluation of early loaded narrow-diameter implants: 3 years follow-up. *Clin Oral Implants Res*, *26*(1), 77-82. doi:10.1111/clr.12281
- Matalova, E., Fleischmannova, J., Sharpe, P. T., & Tucker, A. S. (2008). Tooth agenesis: from molecular genetics to molecular dentistry. *J Dent Res*, *87*(7), 617-623. doi:10.1177/154405910808700715
- McKeown, H. F., Robinson, D. L., Elcock, C., al-Sharood, M., & Brook, A. H. (2002). Tooth dimensions in hypodontia patients, their unaffected relatives and a control group measured by a new image analysis system. *Eur J Orthod*, *24*(2), 131-141. doi:10.1093/ejo/24.2.131
- Nieminen, P., Arte, S., Pirinen, S., Peltonen, L., & Thesleff, I. (1995). Gene defect in hypodontia: exclusion of MSX1 and MSX2 as candidate genes. *Hum Genet*, *96*(3), 305-308. doi:10.1007/bf00210412
- Pjetursson, B. E., Karoussis, I., Bürgin, W., Brägger, U., & Lang, N. P. (2005). Patients' satisfaction following implant therapy. A 10-year prospective cohort study. *Clin Oral Implants Res*, *16*(2), 185-193. doi:10.1111/j.1600-0501.2004.01094.x
- Priest, G. (2019). The treatment dilemma of missing maxillary lateral incisors-Part I: Canine substitution and resin-bonded fixed dental prostheses. *J Esthet Restor Dent*, *31*(4), 311-318. doi:10.1111/jerd.12484
- Qian, L., Todo, M., Matsushita, Y., & Koyano, K. (2009). Effects of implant diameter, insertion depth, and loading angle on stress/strain fields in implant/jawbone systems: finite element analysis. *Int J Oral Maxillofac Implants*, *24*(5), 877-886.
- Rakhshan, V., & Rakhshan, A. (2016). Systematic review and meta-analysis of congenitally missing permanent dentition: Sex dimorphism, occurrence patterns, associated factors and biasing factors. *Int Orthod*, *14*(3), 273-294. doi:10.1016/j.ortho.2016.07.016
- Reddy, M. S., O'Neal, S. J., Haigh, S., Aponte-Wesson, R., & Geurs, N. C. (2008). Initial clinical efficacy of 3-mm implants immediately placed into function in conditions of limited spacing. *Int J Oral Maxillofac Implants*, *23*(2), 281-288.
- Richardson, G., & Russell, K. A. (2001). Congenitally missing maxillary lateral incisors and orthodontic treatment considerations for the single-tooth implant. *J Can Dent Assoc*, *67*(1), 25-28.

- Roccuzzo, A., Imber, J. C., & Jensen, S. S. (2021). Need for lateral bone augmentation at two narrow-diameter implants: A prospective, controlled, clinical study. *Clin Oral Implants Res*, 32(4), 511-520. doi:10.1111/clr.13721
- Roccuzzo, A., Jensen, S. S., Worsaae, N., & Gotfredsen, K. (2020). Implant-supported 2-unit cantilevers compared with single crowns on adjacent implants: A comparative retrospective case series. *J Prosthet Dent*, 123(5), 717-723. doi:10.1016/j.prosdent.2019.04.024
- Roccuzzo, M., Roccuzzo, A., & Ramanuskaite, A. (2018). Papilla height in relation to the distance between bone crest and interproximal contact point at single-tooth implants: A systematic review. *Clin Oral Implants Res*, 29 Suppl 15, 50-61. doi:10.1111/clr.13116
- Sailer, I., Muhlemann, S., Zwahlen, M., Hammerle, C. H., & Schneider, D. (2012). Cemented and screw-retained implant reconstructions: a systematic review of the survival and complication rates. *Clin Oral Implants Res*, 23 Suppl 6, 163-201. doi:10.1111/j.1600-0501.2012.02538.x
- Santing, H. J., Raghoobar, G. M., Vissink, A., den Hartog, L., & Meijer, H. J. (2013). Performance of the Straumann Bone Level Implant system for anterior single-tooth replacements in augmented and nonaugmented sites: a prospective cohort study with 60 consecutive patients. *Clin Oral Implants Res*, 24(8), 941-948. doi:10.1111/j.1600-0501.2012.02486.x
- Schiegnitz, E., & Al-Nawas, B. (2018). Narrow-diameter implants: A systematic review and meta-analysis. *Clin Oral Implants Res*, 29 Suppl 16, 21-40. doi:10.1111/clr.13272
- Shi, J. Y., Xu, F. Y., Zhuang, L. F., Gu, Y. X., Qiao, S. C., & Lai, H. C. (2018). Long-term outcomes of narrow diameter implants in posterior jaws: A retrospective study with at least 8-year follow-up. *Clin Oral Implants Res*, 29(1), 76-81. doi:10.1111/clr.13046
- Thoma, D. S., Cosyn, J., Fickl, S., Jensen, S. S., Jung, R. E., Raghoobar, G. M., . . . Bertl, K. (2021). Soft tissue management at implants: Summary and consensus statements of group 2. The 6th EAO Consensus Conference 2021. *Clin Oral Implants Res*, 32 Suppl 21(Suppl 21), 174-180. doi:10.1111/clr.13798
- Totou, D., Naka, O., Mehta, S. B., & Banerji, S. (2021). Esthetic, mechanical, and biological outcomes of various implant abutments for single-tooth replacement in the anterior region: a systematic review of the literature. *Int J Implant Dent*, 7(1), 85. doi:10.1186/s40729-021-00370-7
- Vastardis, H. (2000). The genetics of human tooth agenesis: new discoveries for understanding dental anomalies. *Am J Orthod Dentofacial Orthop*, 117(6), 650-656.
- Witneben, J. G., Buser, D., Salvi, G. E., Burgin, W., Hicklin, S., & Bragger, U. (2014). Complication and failure rates with implant-supported fixed dental prostheses and single crowns: a 10-year retrospective study. *Clin Implant Dent Relat Res*, 16(3), 356-364. doi:10.1111/cid.12066
- Witneben, J. G., Joda, T., Weber, H. P., & Bragger, U. (2017). Screw retained vs. cement retained implant-supported fixed dental prosthesis. *Periodontol 2000*, 73(1), 141-151. doi:10.1111/prd.12168
- Woelber, J. P., Ratka-Krueger, P., Vach, K., & Frisch, E. (2016). Decementation Rates and the Peri-Implant Tissue Status of Implant-Supported Fixed Restorations Retained via Zinc Oxide Cement: A Retrospective 10-23-Year Study. *Clin Implant Dent Relat Res*, 18(5), 917-925. doi:10.1111/cid.12372
- Zarone, F., Sorrentino, R., Vaccaro, F., & Russo, S. (2006). Prosthetic treatment of maxillary lateral incisor agenesis with osseointegrated implants: a 24-39-month prospective clinical study. *Clin Oral Implants Res*, 17(1), 94-101. doi:10.1111/j.1600-0501.2005.01188.x

Table 1.

Patients and implants characteristics within the two groups (2.9 diameter; 3.3 diameter). Mean (SD) / Number.

	2.9 Ø	3.3 Ø	<i>p</i>
Number of patients/implants	50	50	
Age §	21.2 ± 2.5	21.8 ± 2.8	0.258
Sex (M/F)	17 M, 33 F	24 M, 26 F	0.155
Congenital missing lateral incisor (12; 22)	29 (1.2) 21 (2.2)	23 (1.2) 27 (2.2)	0.230
Length of the implants placed (10; 12 mm)	16 (10 mm) 34 (12 mm)	17 (10 mm) 33 (12 mm)	0.832

M: male,
F: female

Two sample t-test for age and Chi² independence test

Table 2.

Reasons for drop-out

	Ø2.9mm	Ø3.3mm	Total
Deceased	0	1	1
Moved abroad	2	1	3
Withdraw acceptance to participate	1	2	3
<i>Total</i>	3	4	7

Table 3.

Biologic (a) and technical (b) complications within the Ø2.9mm and Ø3.3mm groups at baseline (T1) and 1-year follow-up examination (T2)

<i>a</i>	T1		T2	
	Ø2.9mm	Ø3.3mm	Ø2.9mm	Ø3.3mm
	n=47	n=45	n=47	n=45
Fistula	0 (0%)	0 (0%)	2 (4%)	2 (8%)
Exudation/ suppuration on probing	0 (0%)	0 (0%)	1 (2%)	1 (2%)
Pain	0 (0%)	0 (0%)	0 (0%)	0 (0%)
Necrosis of neighbouring teeth	0 (0%)	0 (0%)	0 (0%)	0 (0%)

<i>b</i>	T1		T2	
	Ø2.9mm	Ø3.3mm	Ø2.9mm	Ø3.3mm
	n=47	n=45	n=47	n=45
Loosening or fracture of abutment screw	0 (0%)	0 (0%)	0 (0%)	1 (2%)
Loss of retention	0 (0%)	0 (0%)	2 (4%)	1 (2%)
Fracture or chipping of veneering ceramic	0 (0%)	0 (0%)	1 (0%)	1 (2%)

Table 4.

Frequency of aesthetic scores within the Ø2.9mm and Ø3.3mm groups at baseline (T1) and 1-year follow-up examination (T2)

		T1		p-value	T2		p-value	T2-T1	
		Ø2.9mm n=47	Ø3.3mm n=45		Ø2.9mm n=47	Ø3.3mm n=45		Ø2.9mm p-value	Ø3.3mm p-value
<i>Symmetry/ harmony</i>	1	39.1%	31.8%	0.769	39.1%	33.3%	0.698	1.000	1.000
	2	41.3%	63.6%		41.3%	61.9%			
	3	19.6%	4.5%		19.6%	4.8%			
<i>Crown morphology</i>	1	69.6%	97.7%	<0.001	69.6%	97.6%	<0.001	1.000	1.000
	2	30.4%	2.3%		30.4%	2.4%			
<i>Crown color</i>	1	50.0%	25.0%	0.006	47.8%	26.2%	0.023	1.000	1.000
	2	50.0%	70.5%		52.2%	71.4%			
	3	0.0%	4.5%		0.0%	2.4%			
<i>Soft tissue color</i>	1	47.8%	43.2%	0.978	39.1%	35.7%	0.747	0.097	0.125
	2	43.5%	56.8%		47.8%	61.9%			
	3	8.7%	0.0%		13.0%	2.4%			
<i>Papilla index (mesial)</i>	1	63.0%	55.8%	0.438	65.2%	73.2%	0.420	1.000	0.146
	2	37.0%	41.9%		34.8%	26.8%			
	3	0.0%	2.3%		0.0%	0.0%			
<i>Papilla index (distal)</i>	1	82.2%	97.6%	0.013	93.3%	100%	0.073	0.063	0.882
	2	17.8%	2.4%		6.7%	0.0%			
<i>Level of the margin</i>	1	69.6%	86.4%	0.049	69.6%	83.3%	0.112	0.882	1.000
	2	30.4%	13.6%		28.3%	16.7%			
	3	0.0%	0.0%		2.2%	0.0%			
<i>Soft tissue texture</i>	1	65.2%	84.1%	0.035	84.8%	92.9%	0.223	0.022	0.125
	2	34.8%	15.9%		15.2%	7.1%			
<i>Soft tissue curvature</i>	1	84.8%	95.5%	0.083	93.5%	95.2%	0.720	0.219	1.000
	2	15.2%	4.5%		6.5%	4.8%			
<i>Alveolar process deficiency</i>	1	71.7%	59.1%	0.182	58.7%	50.0%	0.240	0.031	0.030
	2	28.3%	38.6%		41.3%	40.5%			
	3	0.0%	2.3%		0.0%	9.5%			
<i>Marginal adaptation score</i>	1	89.1%	93.2%	0.492	87.0%	95.2%	0.153	0.280	0.870
	2	6.5%	4.5%		8.7%	4.8%			
	3	4.3%	2.3%		4.3%	0%			
<i>Cement excess (0/1)</i>	No	91.3%	95.5%	0.677	97.8%	97.6%	1.000	0.250	1.000
	Yes	8.7%	4.5%		2.2%	2.4%			

Symmetry/harmony: assessment according to facial midline, tooth axis, contralateral tooth and smile line. Score 1: excellent; score 2: suboptimal but satisfactory; score 3: moderate; score 4: poor symmetry and harmony

Crown morphology: assessment in relation to anatomy, surface texture, contour, prominence, contact points, crown length and crown width in relation to neighboring teeth. Score 1: excellent; score 2: satisfactory, but suboptimal in one or two of the subparameters; score 3: moderate with suboptimal for several subpara-meters; score 4: was poor concerning most of the subparameters

Crown color: assessment according to the hue value, chroma and translucency of the implant-supported crown compared with neighboring teeth. Score 1 excellent color and not easy to distinguish from the natural, neighboring teeth; score 2 was satisfactory, almost optimal but the reconstruction differed from the natural, neighboring teeth; score 3 was moderate, suboptimal color, and score 4 was poor colour match.

Soft tissue score: Score 1: no discoloration, score 2: light greyish discoloration, score 3: distinguishable greyish discoloration, score 4: metal or abutment visible.

Papilla index: Score1: papilla filling the entire proximal space; score 2: papilla filling at least half of the entire proximal space; score 3: papilla filling less than half of the proximal space, score 4: no papilla.

Level of the margin: assessment of the apically or incisally position of the buccal marginal peri-implant mucosa in the middle of the implant crown compared to the contralateral tooth or the neighboring teeth. Score 1: match; score 2: slight mismatch; score 3: moderate mismatch; score 4: mismatch.

Soft tissue texture: assessment related to the smoother or rougher surface texture of the buccal peri-implant mucosa compared to natural gingiva at the contralateral tooth or the neighboring teeth. Score1: match; score 2: slight mismatch; score 3: moderate mismatch; score 4: distinct mismatch.

Soft tissue curvature: assessment according to the over-contoured or under- contoured buccal marginal peri-implant mucosa compared to natural gingiva at the contralateral tooth or the neighboring teeth. Score1: match; score 2: slight mismatch; score 3: moderate mismatch; score 4: distinct mismatch.

Alveolar process deficiency: assessment related to the concavity or convexity of the buccal peri-implant mucosa compared to the natural contour of the buccal gingiva at the contralateral tooth or the neighboring teeth. Score1: match; score 2: slight mismatch; score 3: moderate mismatch; score 4: distinct mismatch.

Marginal adaptation score: radiological assessment of fit or any gap between the implant crown and the abutment mesially and/or distally. Score 1: excellent fit; score 2: distinguishable misfit; score 3: distinct misfit; score 4: unacceptable misfit.

Cement excess: radiographic presence (score 1) or absence (score 0) of cement in relation to the implant crowns

Kendall's Tau-b was used for comparisons between groups

McNemar's test was used for comparisons intra-groups

Table 5.

Patient-reported outcome means of sum scores of questions related to aesthetic outcome, masticatory function, and overall oral health impact on quality of prosthetic treatment, before prosthetic treatment and at 1-year follow-up (T2).

Before prosthetic treatment			T2		
Ø2.9mm	Ø3.3mm	<i>p-value</i>	Ø2.9mm	Ø3.3mm	<i>p-value</i>
10.4 ± 6.00	9.24 ± 6.38	0.382	3.51 ± 5.33	1.76 ± 3.74	0.079

Aesthetic outcome*						
Masticatory function**	3.02 ± 2.76	4.10 ± 3.04	0.093	1.04 ± 1.94	0.86 ± 1.49	0.617
Overall health impact of OHQoL	36.6 ± 25.0	37.9 ± 22.3	0.798	16.9 ± 23.1	10.3 ± 14.2	0.110

*Aesthetic outcome: summary scores of OHIP questions 3, 4, 20, 22, 31, 38

**Functional outcome: summary scores of OHIP questions 1, 28, 29, 32

Two sample t-test

Table 6.

Clinical pre-operative and intra-operative parameters and alveolar process deficiency at T2 in the entire cohort


Mean \pm (SD) / Number (%). Some of the number are mm +/- SD others are n and the parenthesis % please specify


	Alveolar process deficiency			<i>p-value</i>
	Score 1	Score 2	Score 3	
Number of implants	48	36	4	
Width of the alveolar process	8.02 \pm 0.94	8.35 \pm 1.19	7.23 \pm 1.56	0.161
Width of the alveolar ridge	5.51 \pm 1.02	5.63 \pm 0.87	5.15 \pm 0.74	0.555
Thickness facial bone after osteotomy§	1.58 \pm 0.64	1.76 \pm 0.60	1.50 \pm 0.22	0.195
Bone augmentation procedure (yes)	30 (62.5)	14 (38.9)	3 (75.0)	0.032



Score 3 subgroup was excluded from the statistical analysis due to small sample size



Two sample t-test for quantitative variables

Chi² independence test for bone augmentation procedure

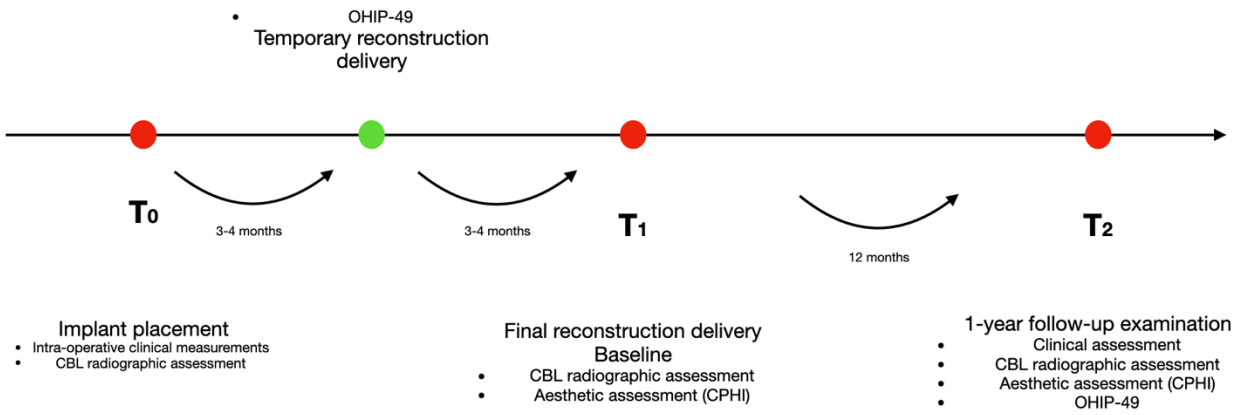

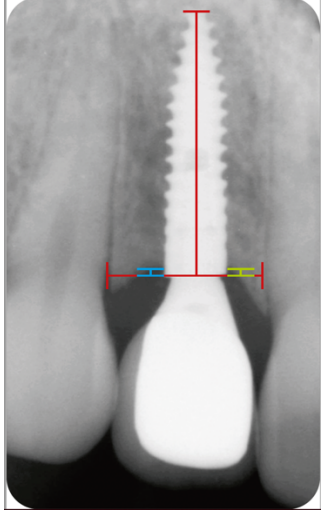

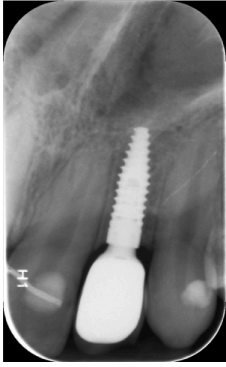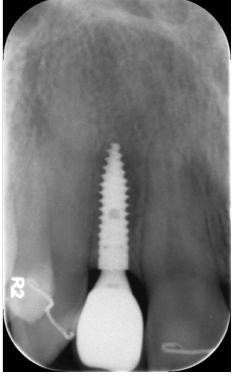

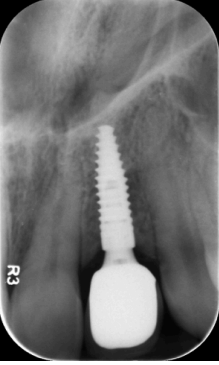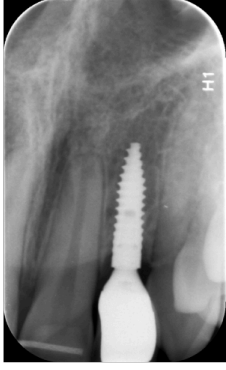

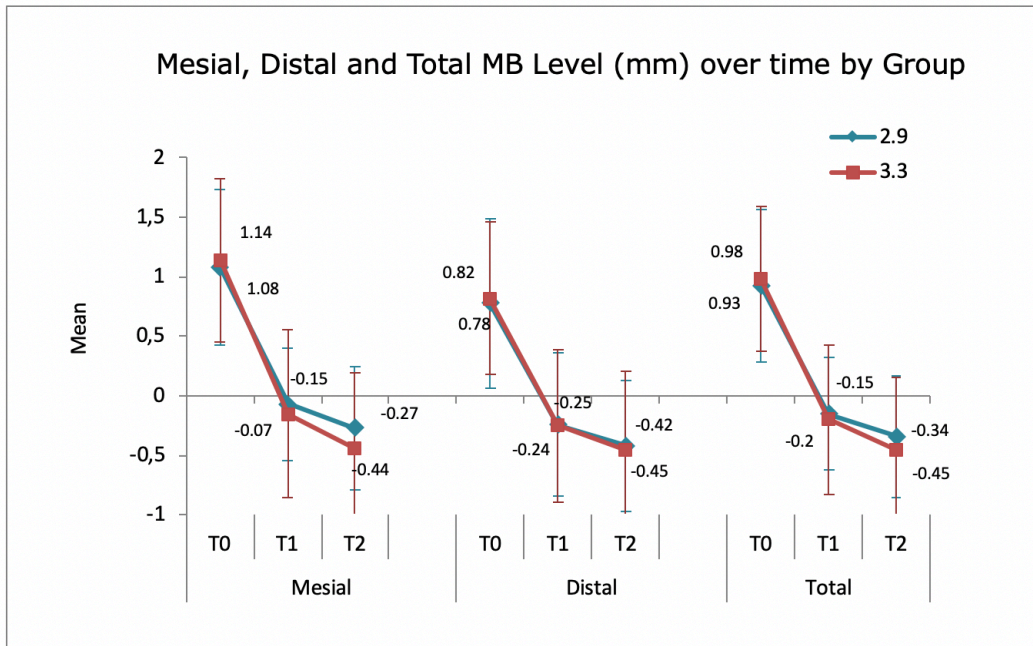


Table 1.

Patients and implants characteristics within the two groups (2.9 diameter; 3.3 diameter). Mean (SD) / Number.

Table 2.

Reasons for drop-out

Table 3.

Biologic (a) and technical (b) complications within the Ø2.9mm and Ø3.3mm groups at baseline (T1) and 1-year follow-up examination (T2)

Table 4.

Frequency of aesthetic scores within the Ø2.9mm and Ø3.3mm groups at baseline (T1) and 1-year follow-up examination (T2)

Table 5.

Patient-reported outcome means of sum scores of questions related to aesthetic outcome, masticatory function, and overall oral health impact on quality of prosthetic treatment, before prosthetic treatment and at 1-year follow-up (T2).

Table 6.

Clinical pre-operative and intra-operative parameters and alveolar process deficiency at T2 in the entire cohort

Mean \pm (SD) / Number (%). Some of the number are mm +/- SD

Figure 1. Study flow-chart

Figure 2. Crestal bone levels were determined by measuring linear distance between the implant shoulder and the first bone to implant contact. The distance is calibrated to the known implant length.

Figure 3. Crestal bone level changes over time within the two groups

Figure 4. Clinical and radiographic presentation of biological and prosthetic complications recorded at the 1-year follow-up: presence of a buccal fistula at the border between keratinized and non-keratinized mucosa (a) and ceramic chipping of the distal incisal edge (b)

Figure 5. Clinical and radiographic presentation of a test (a) and control (b) implant at the 1-year follow-up