

## STATE-OF-THE-ART REVIEW

# Translating Imaging Into 3D Printed Cardiovascular Phantoms



## A Systematic Review of Applications, Technologies, and Validation

Joël Illi, MSc,<sup>a,b,c,\*</sup> Benedikt Bernhard, MD,<sup>a,\*</sup> Christopher Nguyen, PhD,<sup>d,e,f,g</sup> Thomas Pilgrim, MD,<sup>a</sup> Fabien Praz, MD,<sup>a</sup> Martin Gloeckler, MD,<sup>a</sup> Stephan Windecker, MD,<sup>a</sup> Andreas Haeberlin, MD, PhD,<sup>a,c</sup> Christoph Gräni, MD, PhD<sup>a,c</sup>

### HIGHLIGHTS

- 3D printed patient specific phantoms can visualize complex cardiovascular anatomy
- Common imaging modalities for 3D printing are CCT and CMR
- Material jetting/PolyJet and stereolithography are widely used printing techniques
- Standardized validation is warranted to compare different 3D printing technologies

### SUMMARY

Translation of imaging into 3-dimensional (3D) printed patient-specific phantoms (3DPSPs) can help visualize complex cardiovascular anatomy and enable tailoring of therapy. The aim of this paper is to review the entire process of phantom production, including imaging, materials, 3D printing technologies, and the validation of 3DPSPs. A systematic review of published research was conducted using Embase and MEDLINE, including studies that investigated 3DPSPs in cardiovascular medicine. Among 2,534 screened papers, 212 fulfilled inclusion criteria and described 3DPSPs as a valuable adjunct for planning and guiding interventions (n = 108 [51%]), simulation of physiological or pathological conditions (n = 19 [9%]), teaching of health care professionals (n = 23 [11%]), patient education (n = 3 [1.4%]), outcome prediction (n = 6 [2.8%]), or other purposes (n = 53 [25%]). The most common imaging modalities to enable 3D printing were cardiac computed tomography (n = 131 [61.8%]) and cardiac magnetic resonance (n = 26 [12.3%]). The printing process was conducted mostly by material jetting (n = 54 [25.5%]) or stereolithography (n = 43 [20.3%]). The 10 largest studies that evaluated the geometric accuracy of 3DPSPs described a mean bias  $< \pm 1$  mm; however, the validation process was very heterogeneous among the studies. Three-dimensional printed patient-specific phantoms are highly accurate, used for teaching, and applied to guide cardiovascular therapy. Systematic comparison of imaging and printing modalities following a standardized validation process is warranted to allow conclusions on the optimal production process of 3DPSPs in the field of cardiovascular medicine. (J Am Coll Cardiol Basic Trans Science 2022;7:1050-1062) © 2022 The Authors. Published by Elsevier on behalf of the American College of Cardiology Foundation. This is an open access article under the CC BY-NC-ND license (<http://creativecommons.org/licenses/by-nc-nd/4.0/>).

From the <sup>a</sup>Department of Cardiology, University Hospital Bern, Bern, Switzerland; <sup>b</sup>Swiss Med Tech Center, Switzerland Innovation Park Biel/Bienne AG, Biel, Switzerland; <sup>c</sup>Translational Imaging Center, sitem Center for Translational Medicine and Biomedical Entrepreneurship, University of Bern, Bern, Switzerland; <sup>d</sup>Cardiovascular Research Center, Massachusetts General Hospital, Charlestown, Massachusetts, USA; <sup>e</sup>Athinoula A. Martinos Center for Biomedical Imaging, Massachusetts General Hospital, Charlestown, Massachusetts, USA; <sup>f</sup>Department of Medicine, Harvard Medical School, Boston, Massachusetts, USA; and the <sup>g</sup>Division of Health Science Technology, Harvard-Massachusetts Institute of Technology, Cambridge, Massachusetts, USA. \*Mr Illi and Dr Bernhard contributed equally to this work and are joint first authors.

Three-dimensional (3D) printing, also known as additive manufacturing (AM), is an emerging technology that translates images into physical models. 3D printed patient-specific phantoms (3DPSPs) can visualize complex anatomy, provide haptic feedback, and allow personalized training, planning, and tailoring of interventions.<sup>1-3</sup> Recent refinements in the technology, affordable prices, increasing capacity in image acquisition, and advances in postprocessing have contributed to the growing interest and resulted in many studies' reporting the use of 3DPSPs. The manufacturing processes for 3DPSPs encompass image acquisition, image postprocessing, direct or indirect AM, and validation.<sup>4</sup> Compared with other fields of application in which mostly the pure anatomy is of interest and rigid 3DPSPs are applicable (eg, orthopedic surgery), imitation of soft tissue properties (eg, surface texture, dispensability, puncturing behavior, elasticity) and geometric changes during the cardiac cycle constitute an additional challenge in cardiovascular 3DPSPs, especially if phantoms are used for training of surgery or transcatheter interventions. So far, only a few soft materials are available, and no consensus exists on the optimal choice of imaging modalities, printing techniques, and materials, and thus important obstacles remain to the widespread use of cardiovascular 3DPSPs. Recent introduction of new materials, improved 3D printers, and advanced postprocessing techniques might overcome some of these limitations and merit updated review. In this systematic review our aim is to analyze the entire process of 3DPSP production in the field of cardiovascular medicine, including imaging, materials, printing technologies, and validation (Figure 1). Furthermore, current limitations and insights into future directions to improve tissue properties of 3DPSPs are discussed.

## METHODS

Two independent reviewers conducted a systematic review in the databases Embase and MEDLINE, using the search items "3D printing," "3D phantom," "rapid prototyping," or "additive manufacturing" plus 1 of the terms "cardiovascular," "cardiac" or "valve," "left atrial appendage," "aortic," or "coronary arteries." Inclusion criteria were the use of at least one 3DPSP in cardiovascular disease between 2005 and April 2021.

Included studies were checked for cross-references fulfilling the inclusion criteria. Reviews, conference abstracts, editorials, studies of nonpersonalized models, case reports with  $\leq 5$  patients in settings that were previously investigated in larger trials, and bioprinting techniques were excluded (a Consolidated Standards of Reporting Trials flowchart is provided in Figure 2). This review was conducted in accordance with the Preferred Reporting Items for Systematic Reviews and Meta-Analyses statement for reporting systematic reviews.<sup>5</sup>


## RESULTS

A total of 212 studies were included in this systematic review, in which 1,597 3DPSPs were evaluated (Supplemental Table 1). Purposes of 3DPSPs were planning and guiding of cardiovascular interventions (n = 108 [51%]), simulation of physiological or pathological conditions (n = 19 [9%]), teaching of health care professionals (n = 23 [11%]), patient education (n = 3 [1.4%]), evaluation or optimization of 3DPSP manufacturing processes (n = 14 [6.6%]), outcome prediction (n = 6 [2.8%]), other purposes (n = 3 [1.4%]), and proof-of-concept studies to demonstrate the possibility to manufacture 3DPSPs in specific settings (n = 36 [17%]). The number of studies investigating 3DPSPs continuously expanded over the past 16 years, with more than half of the included studies published within the past 4 years (Figure 3). Among the 9 identified randomized controlled trials, 7 were conducted in the field of education and training.<sup>6-12</sup> Results were inconsistent in terms of knowledge gain for students and trainees compared with nonpersonalized models or standard lectures. The only randomized controlled trial investigating the use of 3DPSPs in cardiovascular intervention demonstrated a reduction of intervention time during left atrial appendage occlusion.<sup>13</sup> Across the largest studies, all investigators concluded that the use of 3DPSPs was positive and enhancing in the clinical management of patients with complex geometric cardiovascular conditions.<sup>14-21</sup> Tissue mimicry and poor representation of the cardiac valves were frequently shared concerns, particularly with single-material 3DPSPs.<sup>22</sup>

## ABBREVIATIONS AND ACRONYMS

<b>3D</b>	= 3-dimensional
<b>3DPSP</b>	= 3-dimensional printed patient-specific phantom
<b>AM</b>	= additive manufacturing
<b>CCT</b>	= cardiac computed tomography
<b>CMR</b>	= cardiac magnetic resonance
<b>DICOM</b>	= Digital Imaging and Communications in Medicine
<b>FDM</b>	= fused deposition modeling
<b>PBF</b>	= powder bed fusion
<b>SLA</b>	= stereolithography
<b>TEE</b>	= transesophageal echocardiography
<b>VP</b>	= voxel printing

The authors attest they are in compliance with human studies committees and animal welfare regulations of the authors' institutions and Food and Drug Administration guidelines, including patient consent where appropriate. For more information, visit the [Author Center](#).

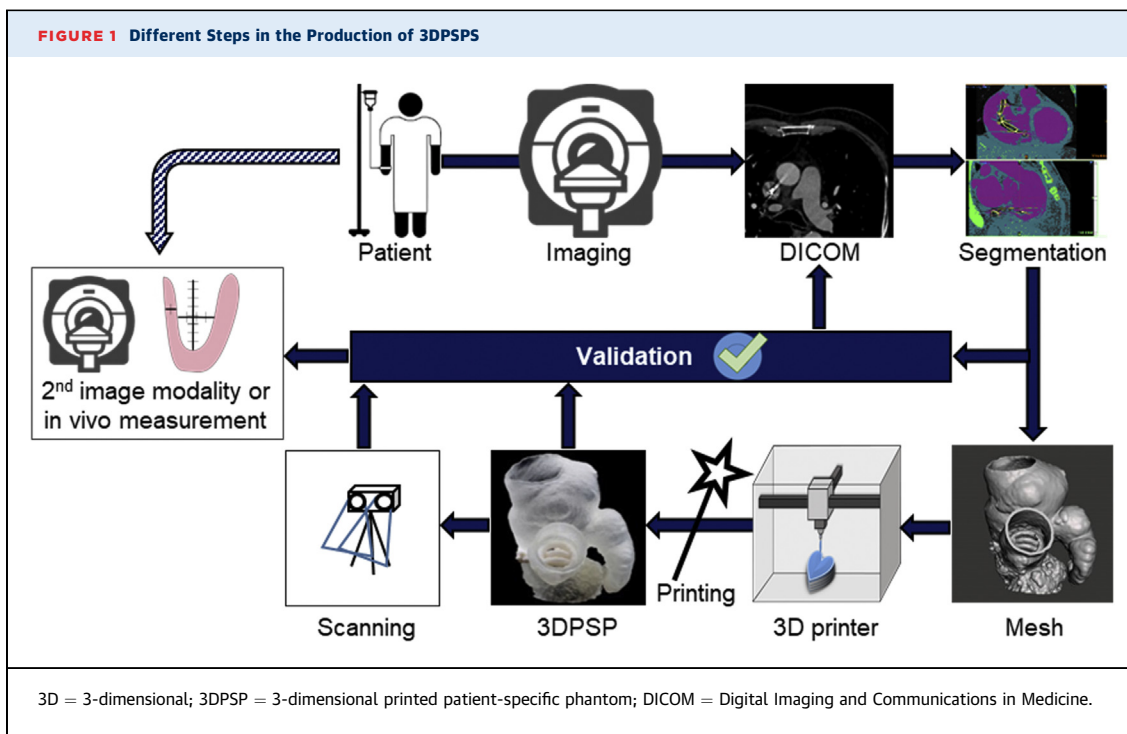


The most common imaging modalities to derive 3DPSPs were cardiac computed tomography (CCT) ( $n = 131$  [61.8%]) and cardiac magnetic resonance (CMR) ( $n = 26$  [12.3%]), whereas 3D transthoracic echocardiography and transesophageal echocardiography (TEE) ( $n = 23$  [10.8%]) and rotational 3D angiography of large vessels ( $n = 2$  [ $<1\%$ ]) were less common. Another 24 studies (11.3%) applied a mixture of modalities across included patients (CCT and CMR,  $n = 21$ ; CCT and 3D TEE,  $n = 2$ ; and CCT, CMR, and 3D TEE,  $n = 1$ ), while 2 studies ( $<1\%$ ) merged data from several modalities; 4 papers (1.9%) did not provide information on the sources of images. Echocardiography-derived 3DPSPs were limited to the depiction of cardiac valves ( $n = 16$ ),<sup>23-34</sup> ventricular or atrial septal defects ( $n = 3$ ),<sup>26,35,36</sup> the left atrial appendage ( $n = 3$ ),<sup>17,37,38</sup> or fetal hearts ( $n = 1$ ).<sup>39</sup>

Across the 166 reviewed studies that provided data about their preferred printing techniques, material jetting, synonymously described using the trade name PolyJet (Stratasys), was the most common printing technology, with 54 papers (25.5%) reporting its exclusive use (**Central Illustration**). Stereolithography (SLA) was the technology of choice in 43 studies (20.3%), whereas fused deposition modeling (FDM), and binder jetting printing were applied in 35 (16.5%) and 13 (8%) studies, respectively. With only 11 papers (5.2%) reporting its use, powder bed fusion (PBF) was the least common AM technology across

the reviewed studies. Ten studies (4.7%) used several printing techniques, and 46 (21.7%) did not provide data on the printing process.

Among the large number of materials available for 3D printing, mostly thermosetting (curing) resins, plastics that solidify irreversibly when the polymeric reaction is initiated, or thermoplastic polymers (plastics that get soft and can be reshaped when heated) were processed. A numeric evaluation of the materials used across studies was not possible, because of the different classification of materials, inconsistent generic terms mixed with brand names, and papers' not providing data on their materials. All studies that applied 3DPSPs in training for interventions ( $n = 8$ ) used soft materials such as silicone ( $n = 4$ )<sup>25,40-42</sup> or PolyJet rubberlike materials (Tango,  $n = 2$ ;<sup>22,43</sup> Agilus,  $n = 2$ ).<sup>44,45</sup> Depending on the purpose of the 3DPSP, different frames across the cardiac cycle were selected. Semilunar valves and ventricles were printed mostly in diastolic frames,<sup>46-48</sup> while for the depiction of atria or atrioventricular valves, systolic or late presystolic frames were chosen.<sup>29,49,50</sup>

Among 54 studies (25%) that evaluated the accuracy of their models, only 15 applied qualitative criteria, and only another 5 validated functional aspects. In the remaining 34 studies, validation processes yielded high variability and included Pearson correlation, mean or median difference or bias, and

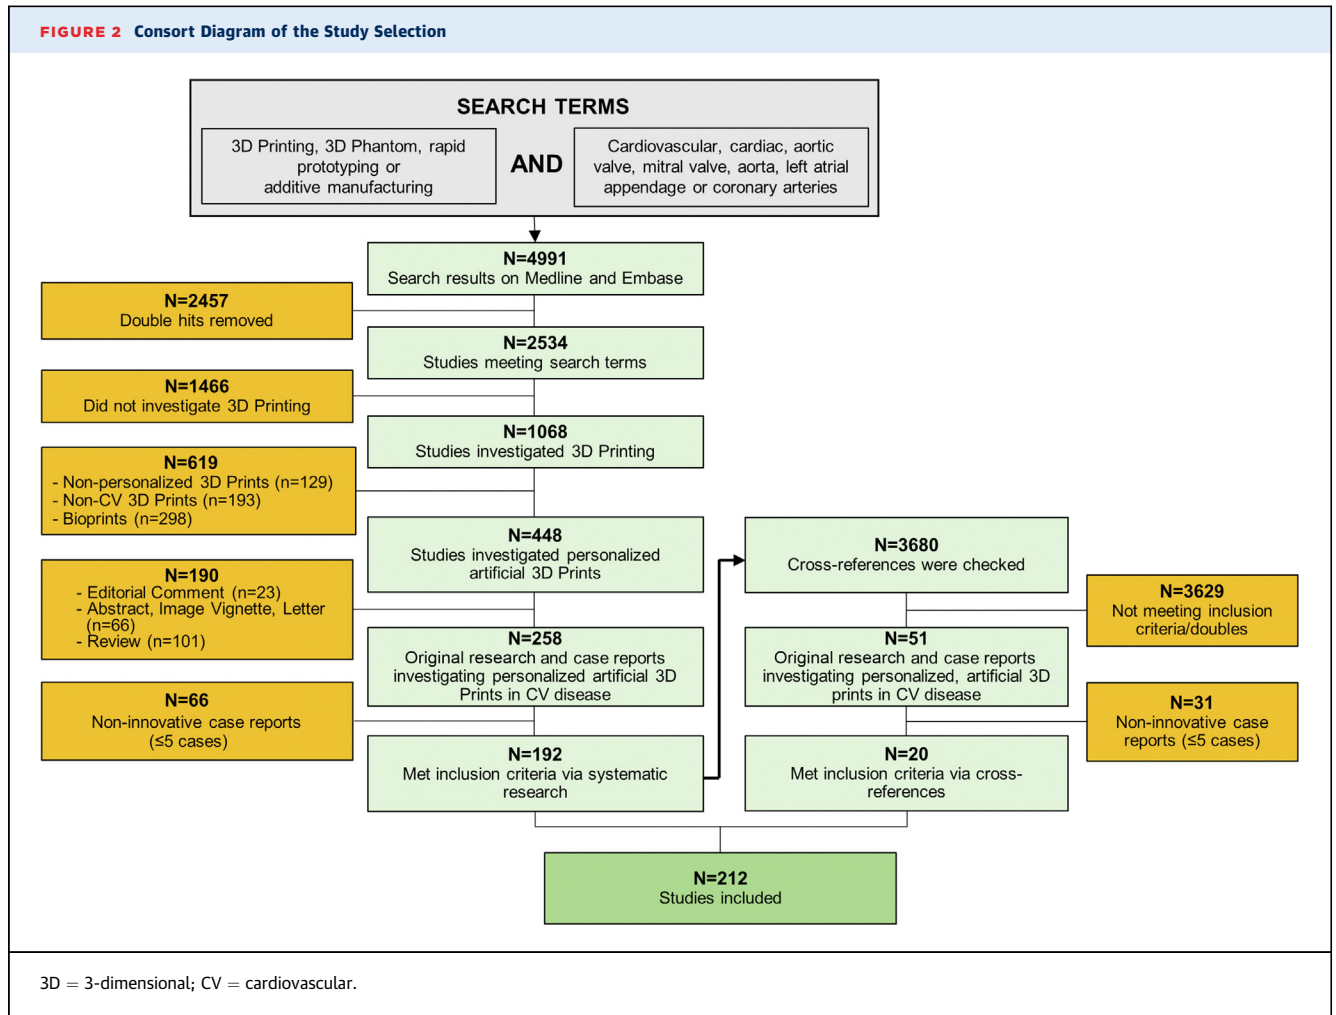


mean error. The number of validated structures ranged from only 1 in each model to complete surface scanning. Original imaging data were mostly chosen as reference standards, while 4 studies used data from other imaging modalities,<sup>13,51-53</sup> and another 4 studies used in vivo findings as a reference standard.<sup>47,52,54,55</sup> Among the 10 largest studies (according to the validated number of 3DPSPs) that evaluated the geometric accuracy of 3DPSP, mean bias was  $< \pm 1$  mm, although heterogeneity in the validation process must be taken into account (Table 1).

## DISCUSSION

Our results demonstrate the current role of 3D printing in cardiovascular medicine, which is so far based on descriptive, observational, and mostly retrospective data, whereas the quantification of the benefit of 3DPSP remains challenging. The manufacturing process for cardiovascular 3DPSPs comprises: 1) imaging

(performed mostly using CCT and CMR); 2) printing (commonly using the PolyJet technique); and 3) validation (with large variation across studies), each of which is discussed in the following sections.

**IMAGE ACQUISITION.** High-resolution imaging modalities that offer the possibility of 3D acquisition are required for AM, which predisposes to CCT and renders it the most commonly used modality. Slice thicknesses of about 1 mm were chosen in most studies, because higher resolutions can go along with higher noise levels, complicating postprocessing and segmentation, although common 3D printers can translate even higher spatial resolution.<sup>3,56</sup> This also applies for small voxel size and sharp kernels.<sup>57</sup> In contrast to CCT, CMR does not expose patients to radiation, which makes it the preferable modality in younger patients. Additional blood pool segmentation with either CMR angiography or 3D balanced steady-state free precession data sets has been shown to be the most accurate method to acquire images for

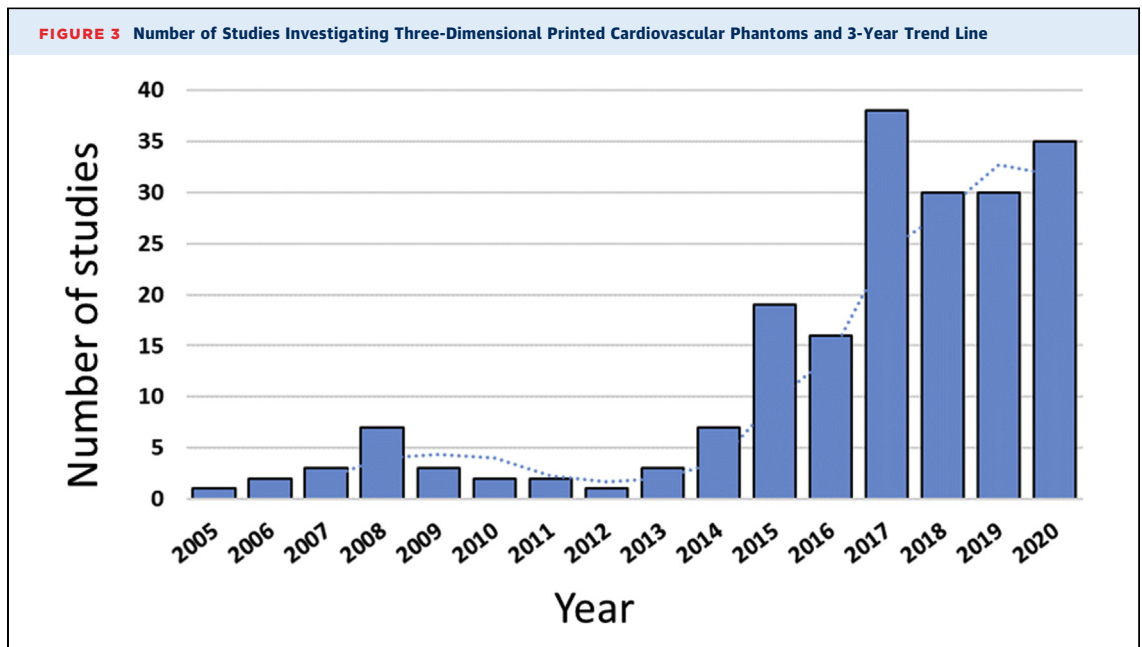


AM by CMR.<sup>46</sup> As demonstrated by Gatti et al,<sup>52</sup> CCT and CMR provide similar accuracy when comparing 3DPSPs with intraoperative findings. Multiplane reconstructions of consecutive high-quality 2-dimensional images have recently made also 3D echocardiography<sup>24,34,58</sup> and rotational 3D angiography of large vessels<sup>59,60</sup> suitable to the requirements of AM.<sup>23</sup> Three-dimensional TEE, as well as 3D transthoracic echocardiography, is widely available, is cost effective, and provides excellent temporal resolution while producing no radiation exposure,<sup>36</sup> although variable reproducibility caused by poor acoustic windows and variations in probe position and acquisition angles are important limitations. High frequencies, going along with higher spatial resolution and harmonic imaging to suppress noise, are beneficial for image quality.<sup>32</sup> However, also under optimal conditions, echocardiography can assess only predefined structures and cannot provide raw data for larger 3DPSPs (ie, models including the ascending and descending parts of the aorta). CCT and CMR offer better blood pool-to-myocardial contrast because of the possibility for contrast agent application,<sup>61</sup> and echocardiographic assessments require extensive postprocessing compared with CCT in specific settings.<sup>50</sup> Similar to echocardiography, rotational angiography is currently a niche application reserved for specific settings of AM, such as printing of malformed vessels.<sup>59,60</sup> Spatial resolution of 0.2 mm was described, allowing detailed and reproducible 3D printing<sup>59</sup> but restricted to the

depiction of hollowed organs with the possibility of contrast agent application and low temporal resolution. More recently, hybrid 3D printing derived from a combination of more than one imaging modality (ie, echocardiography and CCT) has been shown to be a promising technology.<sup>61,62</sup> In fact, fusing and reassembling of 3D data sets from echocardiography and CMR or CCT may allow integration of the strengths of different modalities. So far, experience with this approach is limited to 2 case reports and requires further validation.

Compared with conventional 2-dimensional visualizations of cardiovascular imaging data, 3DPSPs allow in-depth understanding of complex anatomical relationships and therefore allow planning, guiding, and tailoring of cardiovascular therapy and the education of health care professionals.<sup>10</sup> Virtual reality and virtual 3D modeling might challenge 3D printing in terms of visualization of complex anatomy in a user-friendly fashion.<sup>63</sup> However, compared with virtual 3D models, 3DPSPs additionally provide haptic feedback and allow training in practical steps, as demonstrated in several studies.<sup>6-12</sup>

**PRINTER TECHNOLOGIES.** Across the reviewed studies, 5 different technologies were applied for cardiovascular 3D printing, each providing specific strengths and limitations: 1) material jetting (synonymously described as PolyJet); 2) SLA; 3) binder jetting; 4) FDM; and 5) PBF (**Central Illustration**). All technologies use 1 of 2 concepts, a liquid polymer solution that hardens under a specific condition, so-

### CENTRAL ILLUSTRATION Current Techniques to Print 3-Dimensional Cardiovascular Phantoms Across the Reviewed Studies

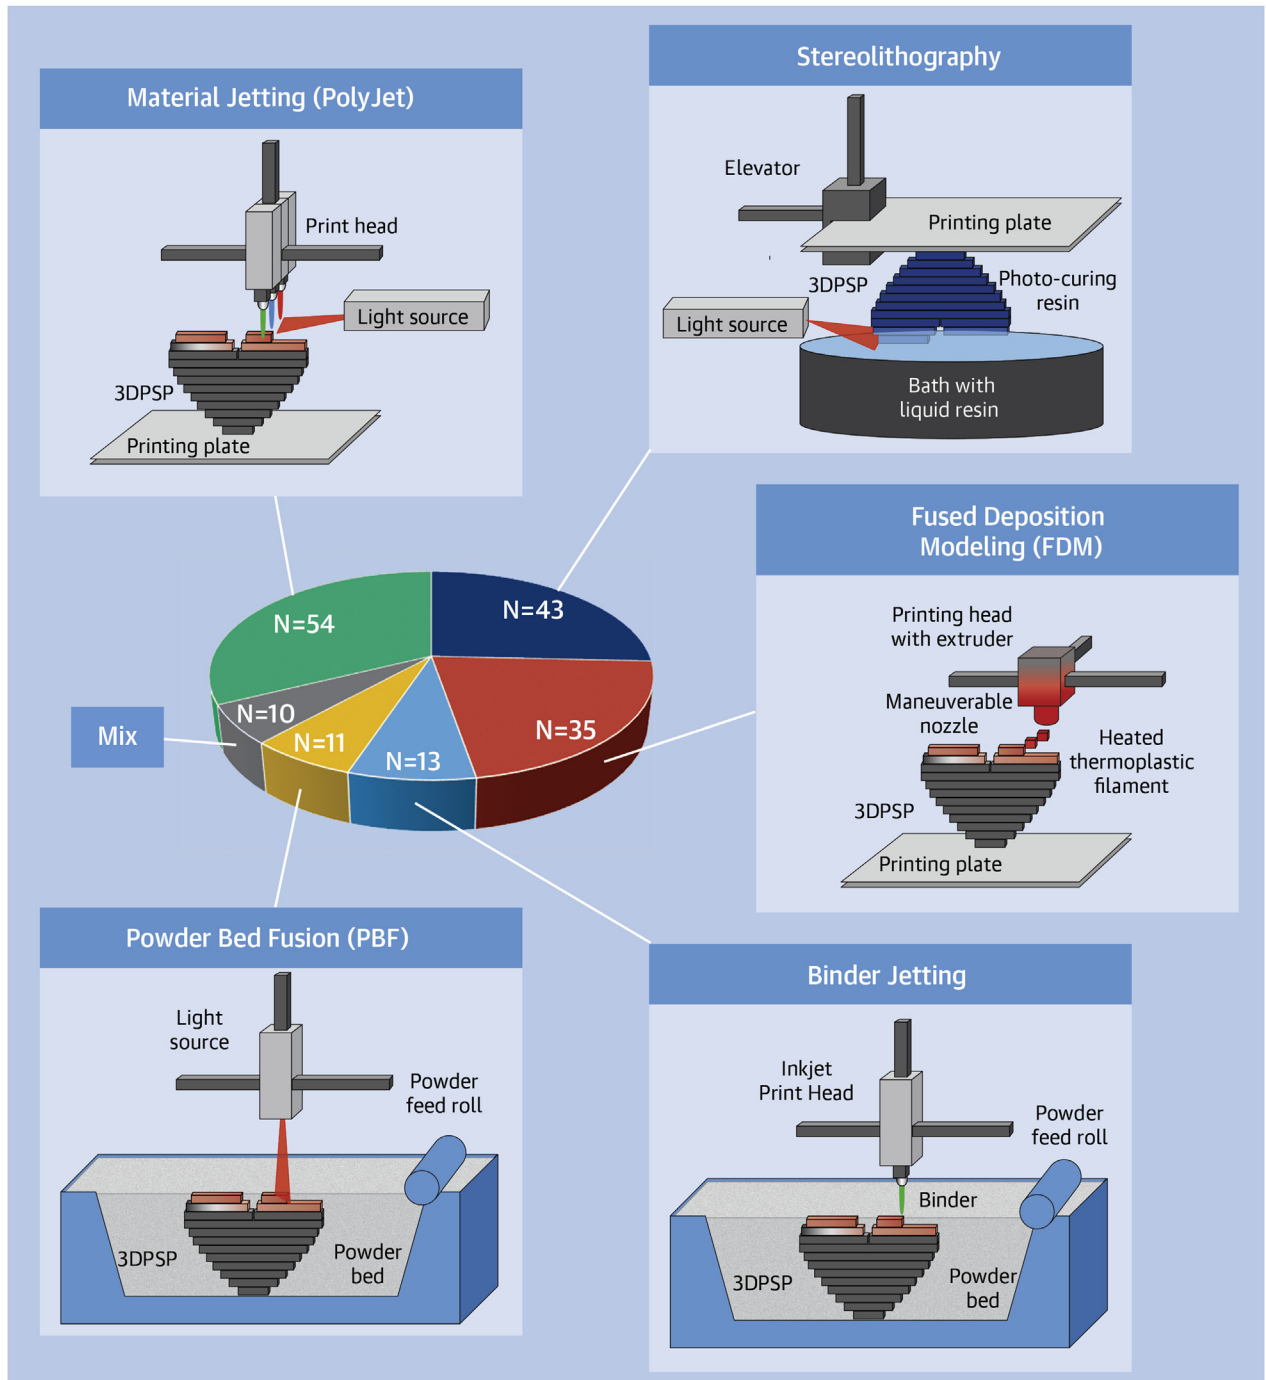

Illi J, et al. J Am Coll Cardiol Basic Trans Science. 2022;7(10):1050-1062.

3DPSP = 3-dimensional printed patient-specific phantom.

**TABLE 1** Selected Studies That Validated 3DPSP Geometric Accuracy

First Author	Number of Validated 3DPSPs	Number of Validated Structures	Validation Technique	Image Modality	Ref. # Standard 1	Correlation Coefficient	Mean Bias, mm ± SD
Dorweiler et al <sup>68</sup>	35	35	Surface congruency	CCT	Deriving image		0.12 ± 0.08
Fan et al <sup>17</sup>	32	96	Dimensions	3D TEE	Deriving image	0.92	-0.1 ± 1.4
Huang et al <sup>39</sup>	30	300	Dimensions	3D TTE	Deriving image		0 ± 0.03
Gatti et al <sup>52</sup>	30	30	Diameters	CMR	CCT	0.92	-0.1 ± 1.1
Valverde et al <sup>16</sup>	20	320	Diameters	CCT/CMR	Deriving image		-0.27 ± 0.73
Faletti et al <sup>47</sup>	20	40	Diameters	CCT	Deriving image	0.96	0.05 ± 0.76
Song et al <sup>38</sup>	18	54	Dimensions	3D TEE	Deriving image	0.92	Maximum 0.4 ± 1.3
Birbara et al <sup>69</sup>	16	NA	Surface distance	CCT	Deriving image		0.13 ± 0.21
Ripley et al <sup>88</sup>	16	16	Diameters	CCT	Deriving image	0.867	-0.34 ± 0.66
Seckeler et al <sup>60</sup>	15	NA	Hausdorff distance	Angiography	Deriving image		0.01 ± 0.003 <sup>a</sup>


<sup>a</sup>Seckeler et al<sup>60</sup> provided mean relative error instead of mean bias.

3D = 3-dimensional; 3DPSP = 3-dimensional printed patient-specific phantom; CCT = cardiac computed tomography; CMR = cardiac magnetic resonance; NA = not available; TEE = transthoracic echocardiography; TTE = transthoracic echocardiography.

called thermosetting polymers (PolyJet, SLA, and binder jetting) or solid thermoplastic polymers that can be melted (FDM and PBF).


Material jetting printing (PolyJet) was the most common printing technique, using a print head depositing layers of a liquid photopolymer on a printing plate that are hardened by UV light.<sup>64</sup> The use of multiple print heads in an array allows the production of complex multimaterial/multicolor 3DPSPs with

modified material properties<sup>65</sup> (Figure 4). PolyJet offers the possibility to process elastic materials such as the commercially available photopolymers Tango, Agilus, and Vero (Stratasys), which provide standardized material properties and were found to yield realistic haptic feedback<sup>22</sup> and hemodynamic properties in simulating aortic valve gradients.<sup>66</sup> Resulting from the excellent spatial resolution of up to 14 μm,<sup>67</sup> PolyJet printed models provide high

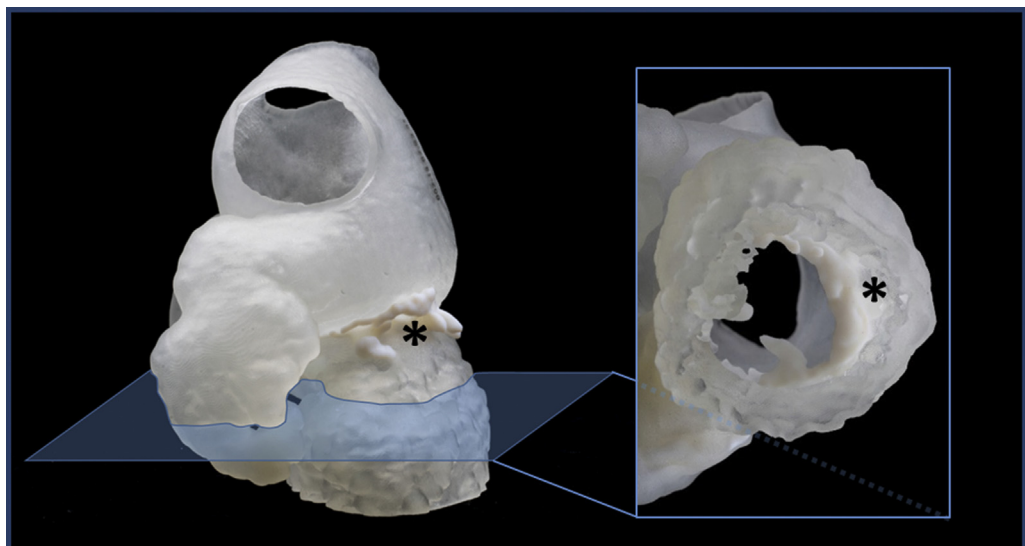**FIGURE 4** Multimaterial 3-Dimensional Printed Patient-Specific Phantom

Cardiac computed tomography-based compliant multimaterial three-dimensional printed patient-specific phantom of the left atrium and aortic root, including mitral annular calcification (asterisk) made by PolyJet printing. Materials: Agilus30 Clear and Agilus30 Clear and Vero Pure White (both Stratasys) mixture for calcifications.

**FIGURE 5** Selected Single-Material 3-Dimensional Printed Patient-Specific Phantom

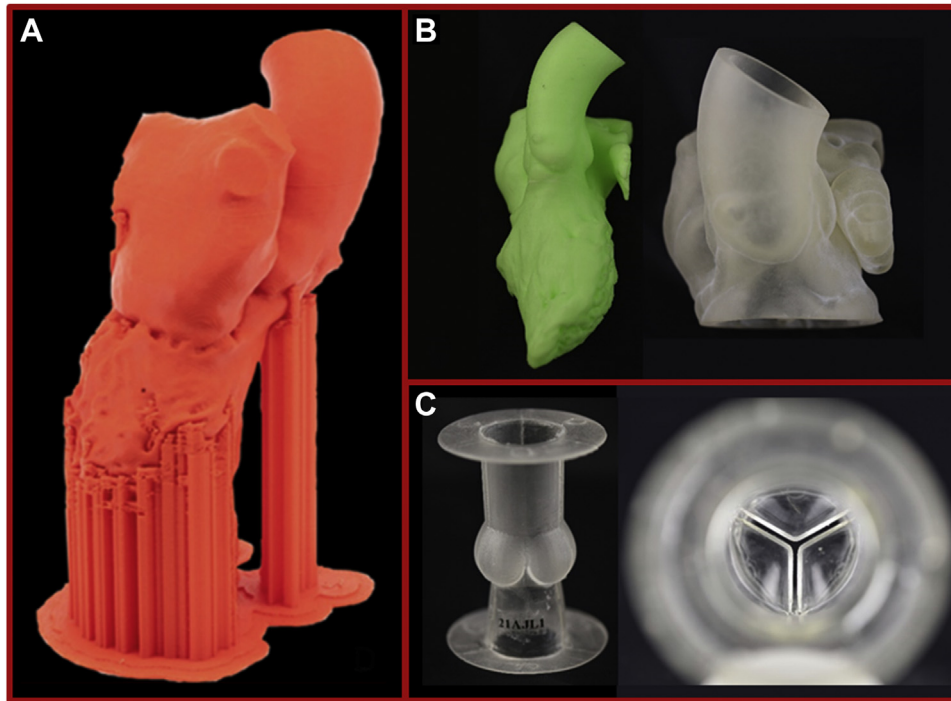

**(A)** Cardiac computed tomography (CCT)-based fused deposition modeling (FDM) positive of the cardiac blood pool, including supporting structures. **(B)** CCT-based cardiac three-dimensional printed patient-specific phantom made from blood pool segmentation with FDM (**green**) or PolyJet (translucent), the latter one with additional adjusted wall thickness. **(C)** Silicone casted (indirect additive manufacturing) aortic root model made from an FDM printed negative.


geometric accuracy.<sup>68,69</sup> Higher costs compared with other techniques and the time intensive nature of the printing process remain relevant limitations.<sup>64</sup>

In SLA printing, a print plate is lowered into a bath containing a thermosetting resin and a photo initiator and then gradually raised to build the model at its bottom. The polymerization process is induced at a desired position by UV light, a laser beam (conventional SLA), or a modulated digital micro mirror device (digital light processing).<sup>70,71</sup> Movement of the printing platform and the light source, as well as the liquid viscosity, define the position of resin solidification.<sup>72</sup> Material properties can be postprocessed using additional light exposition or heating.<sup>73</sup> A variety of photoreactive materials are available for SLA, but the finished model is restricted to be made from a single material.<sup>71</sup> Moreover, SLA materials are usually of higher stiffness compared with PolyJet materials, limiting their value for soft tissue mimicry. Currently, SLA offers spatial resolutions higher than the ones of most imaging modalities, with a maximal resolution of 5  $\mu\text{m}$ .<sup>74</sup>

Binder jetting is another thermosetting technique, closely related to material jetting. In contrary to PolyJet, the inkjet head does not deposit the printing material but a binder that hardens the printing material by displacement on a powder bed.<sup>75,76</sup> This allows the production of rigid models meeting the requirements for use in orthopedic surgery,<sup>77</sup> although they are less suitable for cardiovascular 3DPSPs. Furthermore, binder jetting can produce only single-material models and requires extensive postprocessing.<sup>78</sup>

FDM is a material extrusion technique that heats up and liquefies a thermoplastic filament in an extruder, which is brought on a printing plate through a maneuverable nozzle.<sup>79</sup> Curing of material occurs passively by cooling or by a chemical reaction induced by the head of the extruder. Mechanical properties can be modulated by the choice of materials, layer thickness, orientation of printing filaments, and insertion of air gaps.<sup>80,81</sup> Although rubbery materials are available, FDM printing cannot derive highly compliant 3DPSPs and hence is used

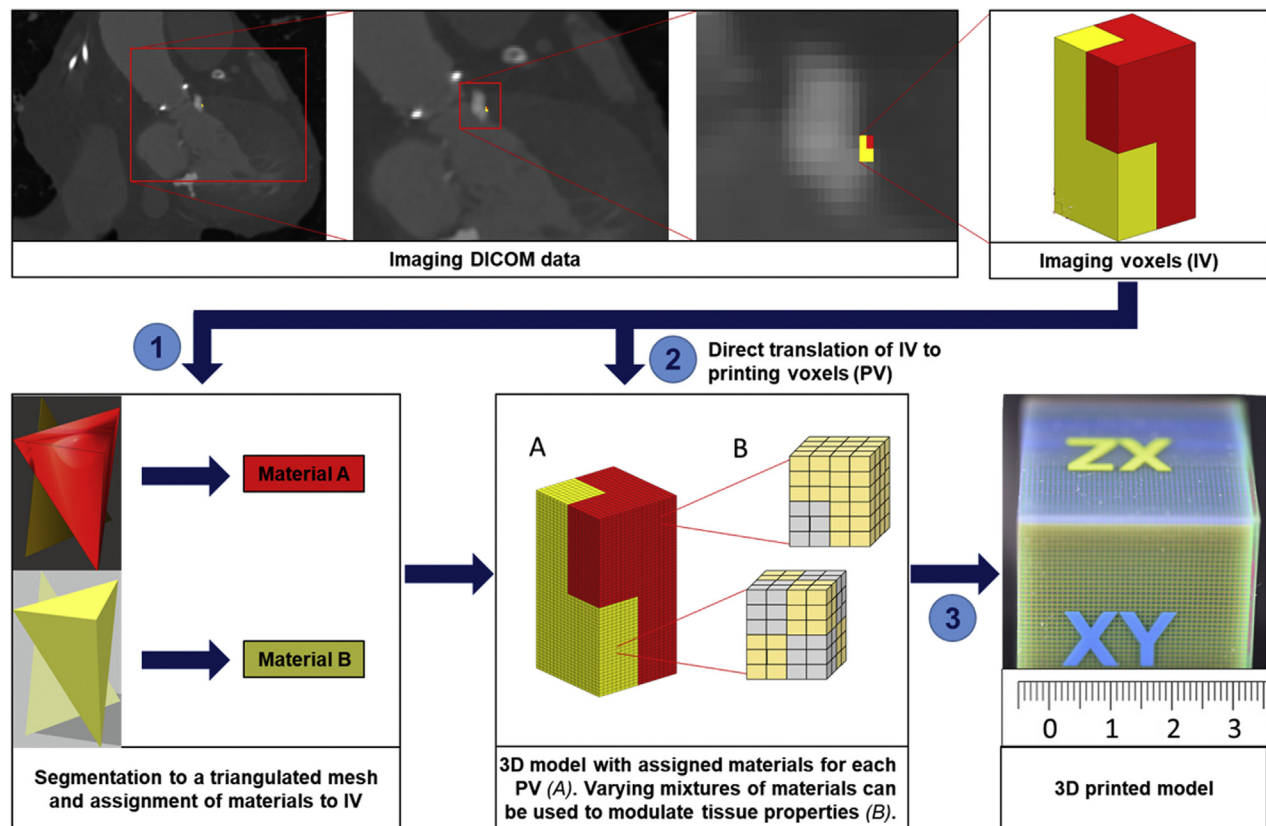

**FIGURE 6** State of the Art Work Flow for 3-Dimensional Printed Patient-Specific Phantom Printing Using Polyjet

On the basis of attenuation values, different masks for different tissues are created in the region of interest. Voxels of the myocardium (red) and aortic valve annular calcification (yellow) are segmented and converted to a triangulated mesh. A specific material is assigned to each voxel type that has been segmented before, eg, solid (yellow) for the calcification and rubber-like (red) for myocardium. Software slices the models and converts them into layer-by-layer commands for the printer. 3D = 3-dimensional; DICOM = Digital Imaging and Communications in Medicine; IV = imaging voxel; PV = printing voxel.

mainly for cast forms or for anatomical models. Spatial resolution relies on the actuation system, the material, user experience, and the geometry of the 3DPSP but is in general lower compared with the previously described modalities. Especially the accuracy of surfaces is a principal concern in FDM printing.<sup>82</sup> Because the material is liquefied, overhanging structures without underlying material support (eg, the roof of a cardiac cavity) are difficult to print and require stabilization of supporting structures (also see [Figure 5A](#)).<sup>57</sup> The low cost of FDM printers and printing materials and its ease of use make FDM widely available, however.<sup>73</sup>

Similar to FDM, PBF is a thermoplastic technique that melts rigid materials (eg, polyamide or thermoplastic polyurethane), which are distributed in a powder bed.<sup>57</sup> The energy source can be a high-power laser (selective laser sintering) or infrared light

(multijet fusion). Material characteristics can be modulated by the laser power, the laser scan speed, and the hatch distance and direction.<sup>78</sup> However, only rigid materials can be processed, limiting the value of PBF for cardiovascular medicine. Furthermore, 3DPSPs usually must be oversized to compensate for material shrinkage during and after the print,<sup>83</sup> and they require postprocessing.<sup>57</sup> The spatial resolution of PBF is adequate for most clinical indications, although structures smaller than 0.5 mm cannot be processed.

The previously mentioned limitations of techniques that derive rigid 3DPSPs (FDM, SLA, and PBF) can be overcome by indirect AM (printing a negative that is processed by casting or brushing to the final 3DPSP). Indirect AM requires laborious further steps besides printing but offers the possibility to derive a large number of nonprintable rubbery materials such

as silicones, more suitable for simulation of cardiac tissue (Figure 5C).<sup>46,49</sup> Silicone rubbers with varying contents of silicone oil can modulate tissue stiffness and were found to provide realistic suture properties in cardiac valve models.<sup>29</sup> However, when directly comparing tissue characteristics of 3DPSPs to those of porcine mitral valve tissue, differences in stiffness and bending modulus are still a relevant concern.<sup>50</sup>

Condensing these findings, we see the value of rigid 3DPSPs that are directly printed using FDM, SLA, PBF, or binder jetting in the visualization of complex anatomical conditions, whereas compliant 3DPSPs from PolyJet printing or indirect AM with silicone casting are applicable for preoperative training and hemodynamic simulations.

**MODEL VALIDATION.** To delineate potential sources of inaccuracy (eg, imaging resolution, accuracy and resolution of segmentation, the resolution of the 3D printer), a comprehensive validation is needed in cardiovascular 3D printing. However, preferred validation methods exhibited large heterogeneity across the reviewed studies or were completely lacking. Apart from qualitative and visual evaluations, the comparison of anatomical structures of 3DPSPs with imaging data as a reference standard was common to validate the geometric accuracy of 3DPSPs. The geometric accuracy described in the reviewed studies can be considered not to pose a relevant limitation for most current clinical applications of 3DPSPs. However, future fields of use, such as tailored devices (eg, valve prostheses or stent grafts adapted to individual vessel geometry) may require higher accuracy and validation of hemodynamic properties before implantation.

In addition to geometric accuracy, evaluation of functional aspects and tissue mimicry are important aspects of validation that should be oriented according to the 3DPSP application. For example, a 3DPSP used for hemodynamic testing requires validation of flow resistance, tensile strength, and dispensability, whereas puncturing behavior, cutting ability, and surface texture are important features in 3DPSPs used for surgical simulations. Several studies have already demonstrated the validation of flow measurements across modulated valves or vessels and reported high accuracy compared with *in vivo* measurements.<sup>33,66,84,85</sup> Tissue characteristics in terms of puncture behavior were adequately replicated in 3DPSPs of the fossa ovalis.<sup>86</sup> However most studies in this field evaluated tissue properties with qualitative or semiquantitative approaches and do not allow generalizations on the optimal choice of

materials and compositions representative of cardiovascular tissue. Systematic *in vitro* testing of material compositions and a standardized validation process for finalized 3DPSPs, including several validation checkpoints, would allow systematic comparison of different materials or printing techniques and could identify optimal manufacturing techniques for cardiovascular 3DPSPs in the future.

## OUTLOOK

Highly accurate 3D printing might allow the production of personalized 3D printed devices such as vascular stent grafts. So far, biocompatibility is an important limitation of implantable devices that might be improved by the introduction of new materials or a combination of conventional 3D printing and bioprinting (eg, conventionally printed synthetic scaffolds coated with biological tissue<sup>87</sup>). Further developments that might increase the use of 3DPSPs are dynamic models that incorporate anatomical and functional changes through the cardiac cycle and the implementation of physiological properties. Voxel printing (VP) is a promising technology in this respect (Figure 6). Compared with current techniques that are limited to a predefined material, VP allows the allocation of a material to each imaging voxel individually. Hence, tissue characteristics can directly be translated into printing voxels without the need for prior segmentation. Even though imaging voxels (spatial resolution in most settings of about 1 mm) in high-resolution imaging are much larger than the printed voxels (spatial resolution of about 80  $\mu\text{m}$ ), printing materials may be mixed and adjusted on a microscopic level to obtain the desired tissue properties. So far, VP is compatible only with PolyJet printing and is not used in clinical cardiovascular applications but might provide 3DPSPs with geometric and mechanical properties similar to human tissue. Furthermore, VP requires a significant amount of technical and medical input, underlining the need to close the gap among clinicians, imaging specialists, and engineers to improve cardiovascular 3D printing.

**STUDY LIMITATIONS.** The reviewed studies included highly selected patient populations and do not allow generalization of observations to all fields of cardiovascular medicine. Despite careful and systematic selection of these studies, specific applications of cardiovascular 3D printing might have been missed in our search, which was based on predefined search terms.

## CONCLUSIONS

Three-dimensional printed cardiovascular phantoms provide sufficient anatomical accuracy for current clinical applications such as the planning, guiding, and tailoring of cardiovascular therapy and the education of health care professionals. As the requirements for 3D models are highly variable, the optimal choice of imaging modalities, printing techniques, and materials as well as their validation so far remains individual to each clinical application. Material jetting and indirect printing with silicone casting can help overcome frequently raised concerns of poor tissue mimicry, whereas directly printed rigid phantoms can visualize complex cardiovascular anatomy. Regarding objectively measurable tissue properties, the incorporation of functional aspects in dynamic models and their comprehensive validation, there is still much room for improvement that could be achieved by VP, contributing to the increased use of 3D printing in the cardiovascular field in the future.

## FUNDING SUPPORT AND AUTHOR DISCLOSURES

Dr Nguyen has received funding from the National Institutes of Health and the American Heart Association. Dr Windecker has received research and educational grants to the institution from Abbott, Amgen, AstraZeneca, Bristol Myers Squibb, Bayer, Biotronik,

Boston Scientific, Cardinal Health, Cardiovalve, CSL Behring, Daiichi Sankyo, Edwards Lifesciences, Guerbet, Infraredx, Johnson and Johnson, Medtronic, Novartis, Polares, OrPha Suisse, Pfizer, Regeneron, Sanofi, Sinomed, Terumo, and V-Wave; serves as an unpaid advisory board member and/or unpaid member of the steering or executive groups of trials funded by Abbott, Abiomed, Amgen, AstraZeneca, Bayer, Bristol Myers Squibb, Boston Scientific, Biotronik, Cardiovalve, Edwards Lifesciences, MedAlliance, Medtronic, Novartis, Polares, Sinomed, Terumo, V-Wave, and Xeltis (but has not received personal payments from pharmaceutical companies or device manufacturers); and is a member of the steering or executive committee groups of several investigator-initiated trials that receive funding from industry, without impact on his personal remuneration. Dr Praz is a consultant for Edwards Lifesciences. Dr Haeberlin has received travel and educational grants from Medtronic and Philips/Spectranetics; is a consultant and advisor for DiNAQOR and Biotronik; and is a cofounder and head of Act-Inno, a device testing company. Dr Pilgrim has received research grants to the institution from Boston Scientific, Edwards Lifesciences, and Biotronik; has received speaker fees from Boston Scientific and Biotronik; is a proctor for Medtronic; and has received reimbursement for travel expenses from Medira. Dr Gräni has received research funding from the Swiss National Science Foundation and Innosuisse, outside the submitted work; and has received travel fees from Amgen and Bayer, outside the submitted work. All other authors have reported that they have no relationships relevant to the contents of this paper to disclose.

**ADDRESS FOR CORRESPONDENCE:** Dr Christoph Gräni, Department of Cardiology, University Hospital Bern-Inselspital Bern, Freiburgstrasse 18, 3010 Bern, Switzerland. E-mail: [christoph.graeni@insel.ch](mailto:christoph.graeni@insel.ch).

## REFERENCES

- Vukicevic M, Mosadegh B, Min JK, Little SH. Cardiac 3D printing and its future directions. *J Am Coll Cardiol Img*. 2017;10:171-184.
- Sun L, Fukuda T, Tokuhara T, Yabuki N. Differences in spatial understanding between physical and virtual models. *Front Architectural Res*. 2014;3:28-35.
- Giannopoulos AA, Mitsouras D, Yoo SJ, Liu PP, Chatzizisis YS, Rybicki FJ. Applications of 3D printing in cardiovascular diseases. *Nat Rev Cardiol*. 2016;13:701-718.
- Chepelev L, Wake N, Ryan J, et al. Radiological Society of North America (RSNA) 3D Printing Special Interest Group (SIG): guidelines for medical 3D printing and appropriateness for clinical scenarios. *3D Print Med*. 2018;4:11.
- Liberati A, Altman DG, Tetzlaff J, et al. The PRISMA statement for reporting systematic reviews and meta-analyses of studies that evaluate health care interventions: explanation and elaboration. *J Clin Epidemiol*. 2009;62:e1-e34.
- Jones TW, Seckeler MD. Use of 3D models of vascular rings and slings to improve resident education. *Congenit Heart Dis*. 2017;12:578-582.
- Lim KH, Loo ZY, Goldie SJ, Adams JW, McMenamin PG. Use of 3D printed models in medical education: a randomized control trial comparing 3D prints versus cadaveric materials for learning external cardiac anatomy. *Anat Sc Educ*. 2016;9:213-221.
- White SC, Sedler J, Jones TW, Seckeler M. Utility of three-dimensional models in resident education on simple and complex intracardiac congenital heart defects. *Congen Heart Dis*. 2018;13:1045-1049.
- Su W, Xiao Y, He S, Huang P, Deng X. Three-dimensional printing models in congenital heart disease education for medical students: a controlled comparative study. *BMC Med Educ*. 2018;18:178.
- Loke YH, Harahsheh AS, Krieger A, Olivieri LJ. Usage of 3D models of tetralogy of Fallot for medical education: impact on learning congenital heart disease. *BMC Med Educ*. 2017;17:54.
- Wang Z, Liu Y, Luo H, Gao C, Zhang J, Dai Y. Is a three-dimensional printing model better than a traditional cardiac model for medical education? A pilot randomized controlled study. *Acta Cardiol Sin*. 2017;33:664-669.
- Ochoa S, Segal J, Garcia N, Fischer EA. Three-dimensional printed cardiac models for focused cardiac ultrasound instruction. *J Ultrasound Med*. 2019;38:1405-1409.
- Li H, Qingyao, Bingshen, et al. Application of 3D printing technology to left atrial appendage occlusion. *Int J Cardiol*. 2017;231:258-263.
- Wang H, Song H, Yang Y, et al. Morphology display and hemodynamic testing using 3D printing may aid in the prediction of LVOT obstruction after mitral valve replacement. *Int J Cardiol*. 2021;331:296-306.
- Biglino G, Capelli C, Wray J, et al. 3D-manufactured patient-specific models of congenital heart defects for communication in clinical practice: feasibility and acceptability. *BMJ Open*. 2015;5:e007165.
- Valverde I, Gomez-Ciriza G, Hussain T, et al. Three-dimensional printed models for surgical planning of complex congenital heart defects: an international multicentre study. *Eur J Cardiothorac Surg*. 2017;52:1139-1148.
- Fan Y, Yang F, Cheung GS, et al. Device sizing guided by echocardiography-based three-dimensional printing is associated with superior outcome after percutaneous left atrial appendage occlusion. *J Am Soc Echocardiogr*. 2019;32:708-719.e1.
- Tong YH, Yu T, Zhou MJ, et al. Use of 3D printing to guide creation of fenestrations in physician-modified stent-grafts for treatment of thoracoabdominal aortic disease. *J Endovasc Ther*. 2020;27:385-393.
- Ryan J, Plasencia J, Richardson R, et al. 3D printing for congenital heart disease: a single site's initial three-year experience. *3D Print Med*. 2018;4:10.

20. Treasure T, Takkenberg JJ, Golesworthy T, et al. Personalised external aortic root support (PEARS) in Marfan syndrome: analysis of 1-9 year outcomes by intention-to-treat in a cohort of the first 30 consecutive patients to receive a novel tissue and valve-conserving procedure, compared with the published results of aortic root replacement. *Heart*. 2014;100:969-975.
21. Andrushchuk U, Adzintsov V, Nivyahlas A, Model H, Ostrovsky Y. Early results of optimal septal myectomy using 3-dimensional printed models. *Kardiochir Torakochirurgia Pol*. 2019;16:74-80.
22. Yoo SJ, Spray T, Austin EH III, Yun TJ, van Arsdell GS. Hands-on surgical training of congenital heart surgery using 3-dimensional print models. *J Thorac Cardiovasc Surg*. 2017;153:1530-1540.
23. Mowers KL, Fullerton JB, Hicks D, Singh GK, Johnson MC, Anwar S. 3D echocardiography provides highly accurate 3d printed models in congenital heart disease. *Pediatr Cardiol*. 2021;42:131-141.
24. Witschey WR, Pouch AM, McGarvey JR, et al. Three-dimensional ultrasound-derived physical mitral valve modeling. *Ann Thorac Surg*. 2014;98:691-694.
25. Engelhardt S, Sauerzapf S, Preim B, Karck M, Wolf I, De Simone R. Flexible and comprehensive patient-specific mitral valve silicone models with chordae tendinae made from 3D-printable molds. *Int J Comput Assist Radiol Surg*. 2019;14:1177-1186.
26. Zhu Y, Liu J, Wang L, et al. Preliminary study of the application of transthoracic echocardiography-guided three-dimensional printing for the assessment of structural heart disease. *Echocardiography*. 2017;34:1903-1908.
27. Sardari Nia P, Heuts S, Daemen J, et al. Preoperative planning with three-dimensional reconstruction of patient's anatomy, rapid prototyping and simulation for endoscopic mitral valve repair. *Interact Cardiovasc Thorac Surg*. 2017;24:163-168.
28. ElGuindy A, Osman A, Elborae A, Nagy M. The utility of 3D printed models in complex percutaneous paravalvular leak interventions. *Glob Cardiol Sci Pract*. 2020;2020:e202027.
29. Premyodhin N, Mandair D, Ferng AS, et al. 3D printed mitral valve models: affordable simulation for robotic mitral valve repair. *Interact Cardiovasc Thorac Surg*. 2018;26:71-76.
30. Heuts S, Daemen JHT, Streukens SAF, et al. Preoperative planning of transapical beating heart mitral valve repair for safe adaptation in clinical practice. *Innovations (Phila)*. 2018;13:200-206.
31. Daemen JHT, Heuts S, Olsthoorn JR, Maessen JG, Sardari Nia P. Mitral valve modelling and three-dimensional printing for planning and simulation of mitral valve repair. *Eur J Cardiothorac Surg*. 2019;55:543-551.
32. Mashari A, Montealegre-Gallegos M, Knio Z, et al. Making three-dimensional echocardiography more tangible: a workflow for three-dimensional printing with echocardiographic data. *Echo Res Pract*. 2016;3:R57-R64.
33. Ginty OK, Moore JT, Eskandari M, et al. Dynamic, patient-specific mitral valve modelling for planning transcatheter repairs. *Int J Comput Assist Radiol Surg*. 2019;14:1227-1235.
34. Herrmann TA, Siefert AW, Pressman GS, et al. In vitro comparison of Doppler and catheter-measured pressure gradients in 3D models of mitral valve calcification. *J Biomech Eng*. 2013;135:94502.
35. Olivieri LJ, Krieger A, Loke YH, Nath DS, Kim PC, Sable CA. Three-dimensional printing of intracardiac defects from three-dimensional echocardiographic images: feasibility and relative accuracy. *J Am Soc Echocardiogr*. 2015;28:392-397.
36. Samuel BP, Pinto C, Pietila T, Vettukattil JJ. Ultrasound-derived three-dimensional printing in congenital heart disease. *J Digit Imaging*. 2015;28:459-461.
37. Liu P, Liu R, Zhang Y, Liu Y, Tang X, Cheng Y. The value of 3D printing models of left atrial appendage using real-time 3D transthoracic echocardiographic data in left atrial appendage occlusion: applications toward an era of truly personalized medicine. *Cardiology*. 2016;135:255-261.
38. Song H, Zhou Q, Zhang L, et al. Evaluating the morphology of the left atrial appendage by a transthoracic echocardiographic 3-dimensional printed model. *Medicine*. 2017;96:e7865.
39. Huang J, Shi H, Chen Q, et al. Three-dimensional printed model fabrication and effectiveness evaluation in fetuses with congenital heart disease or with a normal heart. *J Ultrasound Med*. 2021;40:15-28.
40. Zimmermann JM, Steffen OJ, Vicentini L, et al. Novel augmented physical simulator for the training of transcatheter cardiovascular interventions. *Catheter Cardiovasc Interv*. 2020;95:1202-1209.
41. Hermens JL, Yang R, Burke TM, et al. Development of a 3-D printing-based cardiac surgical simulation curriculum to teach septal myectomy. *J Thorac Cardiovasc Surg*. 2018;156:1139-1148.e3.
42. Abdel-Sayed P, Kalejs M, von Segesser LK. A new training set-up for trans-apical aortic valve replacement. *Interact Cardiovasc Thorac Surg*. 2009;8:599-601.
43. Nam JG, Lee W, Jeong B, et al. Three-dimensional printing of congenital heart disease models for cardiac surgery simulation: evaluation of surgical skill improvement among inexperienced cardiothoracic surgeons. *Kor J Radiol*. 2021;22:706-713.
44. Hussein N, Honjo O, Haller C, et al. Quantitative assessment of technical performance during hands-on surgical training of the arterial switch operation using 3-dimensional printed heart models. *J Thorac Cardiovasc Surg*. 2020;160:1035-1042.
45. Hussein N, Honjo O, Barron DJ, Haller C, Coles JG, Yoo SJ. The incorporation of hands-on surgical training in a congenital heart surgery training curriculum. *Ann Thorac Surg*. 2021;112:1672-1680.
46. Farooqi KM, Lengua CG, Weinberg AD, Nielsen JC, Sanz J. Blood pool segmentation results in superior virtual cardiac models than myocardial segmentation for 3D printing. *Pediatr Cardiol*. 2016;37:1028-1036.
47. Faletti R, Gatti M, Cosentino A, et al. 3D printing of the aortic annulus based on cardiovascular computed tomography: preliminary experience in pre-procedural planning for aortic valve sizing. *J Cardiovasc Comput Tomogr*. 2018;12:391-397.
48. Perens G, Chyu J, McHenry K, Yoshida T, Finn JP. Three-dimensional congenital heart models created with free software and a desktop printer: assessment of accuracy, technical aspects, and clinical use. *World J Pediatr Congen Heart Surg*. 2020;11:797-801.
49. Scanlan AB, Nguyen AV, Ilina A, et al. Comparison of 3D echocardiogram-derived 3D printed valve models to molded models for simulated repair of pediatric atrioventricular valves. *Pediatr Cardiol*. 2018;39:538-547.
50. Vukicevic M, Puperi DS, Jane Grande-Allen K, Little SH. 3D printed modeling of the mitral valve for catheter-based structural interventions. *Ann Biomed Eng*. 2017;45:508-519.
51. Matsubara D, Kataoka K, Takahashi H, Minami T, Yamagata T. A patient-specific hollow three-dimensional model for simulating percutaneous occlusion of patent ductus arteriosus. *Int Heart J*. 2019;60:100-107.
52. Gatti M, Cosentino A, Cura Stura E, et al. Accuracy of cardiac magnetic resonance generated 3D models of the aortic annulus compared to cardiovascular computed tomography generated 3D models. *Int J Cardiovasc Imaging*. 2020;36:2007-2015.
53. Valverde I, Gomez G, Coserria JF, et al. 3D printed models for planning endovascular stenting in transverse aortic arch hypoplasia. *Catheter Cardiovasc Interv*. 2015;85:1006-1012.
54. Olejnik P, Nosal M, Havran T, et al. Utilisation of three-dimensional printed heart models for operative planning of complex congenital heart defects. *Kardiologia Pol*. 2017;75:495-501.
55. Ma XJ, Tao L, Chen X, et al. Clinical application of three-dimensional reconstruction and rapid prototyping technology of multislice spiral computed tomography angiography for the repair of ventricular septal defect of tetralogy of Fallot. *Genet Mol Res*. 2015;14:1301-1309.
56. Tuncay V, van Ooijen PMA. 3D printing for heart valve disease: a systematic review. *Eur Radiol Exp*. 2019;3:9.
57. Otton JM, Birbara NS, Hussain T, Greil G, Foley TA, Pather N. 3D printing from cardiovascular CT: a practical guide and review. *Cardiovasc Diagn Ther*. 2017;7:507-526.
58. Mahmood F, Owais K, Montealegre-Gallegos M, et al. Echocardiography derived three-dimensional printing of normal and abnormal mitral annuli. *Ann Card Anaesth*. 2014;17:279-283.
59. Parimi M, Buelter J, Thanugundla V, et al. Feasibility and validity of printing 3D heart models

- from rotational angiography. *Pediatr Cardiol.* 2018;39:653–658.
60. Seckeler MD, Boe BA, Barber BJ, Berman DP, Armstrong AK. Use of rotational angiography in congenital cardiac catheterisations to generate three-dimensional-printed models. *Cardiol Young.* 2021;31:1407–1411.
61. Gosnell J, Pietila T, Samuel BP, Kurup HK, Haw MP, Vettukattil JJ. Integration of computed tomography and three-dimensional echocardiography for hybrid three-dimensional printing in congenital heart disease. *J Digit Imaging.* 2016;29:665–669.
62. Gomez A, Gomez G, Simpson J, Valverde I. 3D hybrid printed models in complex congenital heart disease: 3D echocardiography and cardiovascular magnetic resonance imaging fusion. *Eur Heart J.* 2020;41:4214.
63. Lau I, Gupta A, Sun Z. Clinical value of virtual reality versus 3d printing in congenital heart disease. *Biomolecules.* 2021;11:884.
64. Bandyopadhyay A, Heer B. Additive manufacturing of multi-material structures. *Mater Sci Eng Rep.* 2018;129:1–16.
65. Ionita CN, Mokin M, Varble N, et al. Challenges and limitations of patient-specific vascular phantom fabrication using 3D PolyJet printing. *Proc SPIE.* 2014;9038:90380m.
66. Maragiannis D, Jackson MS, Igo SR, et al. Replicating patient-specific severe aortic valve stenosis with functional 3D modeling. *Circ Cardiovasc Imaging.* 2015;8:e003626.
67. Yun Lu T, Peng C, Pille P, Leary M, Tran JP. PolyJet 3D printing of composite materials: experimental and modelling approach. *J Miner Metals Mater Soc.* 2020;72:13.
68. Dorweiler B, Baqué PE, Chaban R, Ghazy A, Salem O. Quality control in 3D printing: accuracy analysis of 3D-printed models of patient-specific anatomy. *Materials (Basel).* 2021;14:1021.
69. Birbara NS, Otton JM, Pather N. 3D modelling and printing technology to produce patient-specific 3D models. *Heart Lung Circ.* 2019;28:302–313.
70. Binder TM, Moertl D, Mundigler G, et al. Stereolithographic biomodeling to create tangible hard copies of cardiac structures from echocardiographic data: in vitro and in vivo validation. *J Am Coll Cardiol.* 2000;35:230–237.
71. Melchels FPW, Feijen J, Grijpma DW. A review on stereolithography and its applications in biomedical engineering. *Biomaterials.* 2010;31:6121–6130.
72. Mankovich NJ, Cheeseman AM, Stoker NG. The display of three-dimensional anatomy with stereolithographic models. *J Digit Imaging.* 1990;3:200.
73. Ngo TD, Kashani A, Imbalzano G, Nguyen KTQ, Hui D. Additive manufacturing (3D printing): a review of materials, methods, applications and challenges. *Composites B Eng.* 2018;143:172–196.
74. Huang J. A review of stereolithography: processes and systems. *Processes.* 2020;8:1138.
75. Castro-Sastre MÁ, Fernández-Abia AI, Piep J, Rodríguez-González P, Barreiro J. Towards functional parts by binder jetting calcium-sulphate with thermal treatment post-processing. *Materials (Basel).* 2020;13:3818.
76. Salmi M. Additive manufacturing processes in medical applications. *Materials (Basel).* 2021;14:191.
77. Tai BL, Kao YT, Payne N, Zheng Y, Chen L, Shih AJ. 3D printed composite for simulating thermal and mechanical responses of the cortical bone in orthopaedic surgery. *Med Eng Phys.* 2018;61:61–68.
78. Gokuldoss PK, Kolla S, Eckert J. Additive manufacturing processes: selective laser melting, electron beam melting and binder jetting-selection guidelines. *Materials (Basel).* 2017;10:672.
79. Mohamed OA, Masood SH, Bhowmik JL. Optimization of fused deposition modeling process parameters: a review of current research and future prospects. *Adv Manuf.* 2015;3:42–53.
80. Lee BH, Abdullah J, Khan ZA. Optimization of rapid prototyping parameters for production of flexible ABS object. *J Mater Process Technol.* 2005;169:54–61.
81. Abdullah J, Khan Z, Khu SY. Optimizing flexible behaviour of bow prototype using Taguchi approach. *J Appl Sci.* 2006;6.
82. Chohan JS, Singh R, Boparai KS, Penna R, Fraternali F. Dimensional accuracy analysis of coupled fused deposition modeling and vapour smoothing operations for biomedical applications. *Composites B Eng.* 2017;117:138–149.
83. Berry E, Brown JM, Connell M, et al. Preliminary experience with medical applications of rapid prototyping by selective laser sintering. *Med Eng Phys.* 1997;19:90–96.
84. Medero R, García-Rodríguez S, François CJ, Roldán-Alzate A. Patient-specific in vitro models for hemodynamic analysis of congenital heart disease—additive manufacturing approach. *J Biomechanics.* 2017;54:111–116.
85. Canstein C, Cachot P, Faust A, et al. 3D MR flow analysis in realistic rapid-prototyping model systems of the thoracic aorta: comparison with in vivo data and computational fluid dynamics in identical vessel geometries. *Magn Reson Med.* 2008;59:535–546.
86. Bezek LB, Cauchi MP, De Vita R, Foerst JR, Williams CB. 3D printing tissue-mimicking materials for realistic transeptal puncture models. *J Mech Behav Biomed Mater.* 2020;110:103971.
87. Carrabba M, Madeddu P. Current strategies for the manufacture of small size tissue engineering vascular grafts. *Front Bioeng Biotechnol.* 2018;6:41.
88. Ripley B, Kelil T, Cheezum MK, et al. 3D printing based on cardiac CT assists anatomic visualization prior to transcatheter aortic valve replacement. *J Cardiovasc Comput Tomogr.* 2016;10:28–36.

---

**KEY WORDS** 3D printing, additive manufacturing, cardiovascular disease, patient-specific phantoms, personalized medicine, silicone casting, voxel printing

---

**APPENDIX** For a supplemental table, please see the online version of this paper.