

Multi Frequency Phase Fluorimetry (MFPF) for Oxygen Partial Pressure Measurement: *Ex Vivo* Validation by Polarographic Clark-Type Electrode

Stefan Boehme^{1,2*}, Bastian Duenges², Klaus U. Klein^{1,2}, Volker Hartwich⁴, Beate Mayr⁵, Jolanda Consiglio⁵, James E. Baumgardner³, Klaus Markstaller^{1,2}, Reto Basciani⁴, Andreas Vogt⁴

1 Department of Anaesthesia, General Intensive Care and Pain Management, Medical University of Vienna, Vienna, Austria, **2** Department of Anesthesiology, Medical Center of the Johannes Gutenberg-University, Mainz, Germany, **3** Oscillogy, Folsom, Pennsylvania, United States of America, **4** Department of Anesthesiology and Pain Therapy, Inselspital, Bern University Hospital, and University of Bern, Bern, Switzerland, **5** Department of Cardiovascular Surgery, Swiss Cardiovascular Center, Bern University Hospital, Bern, Switzerland

Abstract

Background: Measurement of partial pressure of oxygen (P_{O_2}) at high temporal resolution remains a technological challenge. This study introduces a novel P_{O_2} sensing technology based on Multi-Frequency Phase Fluorimetry (MFPF). The aim was to validate MFPF against polarographic Clark-type electrode (CTE) P_{O_2} measurements.

Methodology/Principal Findings: MFPF technology was first investigated in $N=8$ anaesthetised pigs at F_{IO_2} of 0.21, 0.4, 0.6, 0.8 and 1.0. At each F_{IO_2} level, blood samples were withdrawn and P_{O_2} was measured *in vitro* with MFPF using two FOXY-AL300 probes immediately followed by CTE measurement. Secondly, MFPF- P_{O_2} readings were compared to CTE in an artificial circulatory setup (human packed red blood cells, haematocrit of 30%). The impacts of temperature (20, 30, 40°C) and blood flow (0.8, 1.6, 2.4, 3.2, 4.0 L min⁻¹) on MFPF- P_{O_2} measurements were assessed. MFPF response time in the gas- and blood-phase was determined. Porcine MFPF- P_{O_2} ranged from 63 to 749 mmHg; the corresponding CTE samples from 43 to 712 mmHg. Linear regression: CTE = 15.59 + 1.18 * MFPF ($R^2=0.93$; $P<0.0001$). Bland Altman analysis: mean_{diff} 69.2 mmHg, range_{diff} -50.1/215.6 mmHg, 1.96-SD limits -56.3/194.8 mmHg. In artificial circulatory setup, MFPF- P_{O_2} ranged from 20 to 567 mmHg and CTE samples from 11 to 575 mmHg. Linear regression: CTE = -8.73 + 1.05 * MFPF ($R^2=0.99$; $P<0.0001$). Bland-Altman analysis: mean_{diff} 6.6 mmHg, range_{diff} -9.7/20.5 mmHg, 1.96-SD limits -12.7/25.8 mmHg. Differences between MFPF and CTE- P_{O_2} due to variations of temperature were less than 6 mmHg (range 0–140 mmHg) and less than 35 mmHg (range 140–750 mmHg); differences due to variations in blood flow were less than 15 mmHg (all P -values > 0.05). MFPF response-time (monoexponential) was 1.48 ± 0.26 s for the gas-phase and 1.51 ± 0.20 s for the blood-phase.

Conclusions/Significance: MFPF-derived P_{O_2} readings were reproducible and showed excellent correlation and good agreement with Clark-type electrode-based P_{O_2} measurements. There was no relevant impact of temperature and blood flow upon MFPF- P_{O_2} measurements. The response time of the MFPF FOXY-AL300 probe was adequate for real-time sensing in the blood phase.

Citation: Boehme S, Duenges B, Klein KU, Hartwich V, Mayr B, et al. (2013) Multi Frequency Phase Fluorimetry (MFPF) for Oxygen Partial Pressure Measurement: *Ex Vivo* Validation by Polarographic Clark-Type Electrode. PLoS ONE 8(4): e60591. doi:10.1371/journal.pone.0060591

Editor: Randen Lee Patterson, UC Davis School of Medicine, United States of America

Received: December 18, 2012; **Accepted:** February 28, 2013; **Published:** April 2, 2013

Copyright: © 2013 Boehme et al. This is an open-access article distributed under the terms of the Creative Commons Attribution License, which permits unrestricted use, distribution, and reproduction in any medium, provided the original author and source are credited.

Funding: The study was supported by research grants of the German Research Council (DFG PAK 415/7-1, Ma 2398-3) and Swiss National Foundation (SNF POIB 117065/1), and by an institutional grant of the Research Department of Anesthesiology and Pain Therapy, Inselspital, Bern, Switzerland. The funders had no role in study design, data collection and analysis, decision to publish, or preparation of the manuscript.

Competing Interests: JEB is President of Fa. Oscillogy. RB received lecture honoraria from Medtronic Switzerland for lectures in the field of anesthetic management for transcatheter aortic valve implantation. RB received lecture honoraria and a travel grant from Covidien Europe for speaking at the meeting of the European Association of Cardiothoracic Anaesthesiologists (EACTA) in the field of near-infrared spectroscopy for cerebral tissue oximetry in thoracic aortic surgery. In the authors' opinion, these conflicts are in no way related to being competitive in the field of our manuscript: these conflicts do not interfere with, or could be perceived as interfering with, the complete and objective presentation, peer review, editorial decision-making, or publication of the manuscript. There are no conflicts related to being competitive researchers in this field. Overall, this does not alter the authors' adherence to all the PLOS ONE policies on sharing data and materials.

* E-mail: stefan_boehme@web.de

Introduction

The polarographic Clark-type electrode remains the gold standard for oxygen partial pressure (P_{O_2}) measurement to date, and is the underlying electrochemical principle of conventional blood gas P_{O_2} analysis [1,2,3,4]. Moreover, polarographic P_{O_2}

probes, such as the Licox probe, are used for the continuous monitoring of oxygen. These probes provide favourable properties, including high accuracy and stability; however, they lack high temporal resolution [5]. Several publications reveal that oxygen levels may largely fluctuate over time in the systemic (e.g., thoracic aorta) or capillary circulation (e.g. vasomotion, brain resting state)

[6,7,8,9,10] due to oxygen consumption and delivery. Therefore, novel, fast oxygen-sensing technologies are required for the investigation of these physiologic or pathophysiologic phenomena [11,12].

Recently, a novel technology for fast oxygen sensing based on Multi Frequency Phase Fluorimetry (MFPF), termed NeoFox® (OceanOptics, Dunedin, USA; www.oceanoptics.com), was released. This technology is suitable for 10 Hz oxygen measurements using fluorescent dye sensors such as the FOXY-AL300 (OceanOptics, Dunedin, USA). This indwelling, uncoated ruthenium tipped fibre optic probe allows for rapid measurement of oxygen within blood or tissue. The technology, however, has not yet been compared to conventional polarographic Clark-type electrode (CTE)-based P_{O₂} measurements [13,14].

This study aimed to validate MFPF-P_{O₂} measurements versus CTE-based measurements of oxygen partial pressure. Firstly, in a porcine lung model, MFPF-P_{O₂} was measured *in vitro* without the interference of blood flow using two FOXY-AL300 probes (OceanOptics, Dunedin, USA) and was then compared to CTE blood gas P_{O₂} analysis. Secondly, for further validation, we developed an artificial extracorporeal circulation setup primed with a mixture of crystalloid, colloid and human packed red cells to imitate *in vivo* conditions. In this setup, MFPF-P_{O₂} readings were assessed and then compared to conventionally measured P_{O₂} by CTE. Furthermore, in the artificial circulation setup, temperature and blood flow were randomly varied in order to evaluate their impact on MFPF-P_{O₂} measurements. In addition, MFPF FOXY-AL300 (OceanOptics, Dunedin, USA) probe response times were determined in the gas- and blood-phases to further assess this novel technology. In summary, the overall aim could be achieved.

Materials and Methods

MFPF Technological Principle

The MFPF platform (NeoFox®, OceanOptics, Dundin, USA) was mounted with the indwelling FOXY-AL300 (OceanOptics, Dunedin, USA) aluminium-jacketed optical fibre probe (500 μm outer and 300 μm core diameter) with an uncoated ruthenium complex at the tip to assess luminescence lifetime in the region surrounding the fluorescent dye, which was roughly equal to the fibre-optic tip surface area (about 0.3 mm²). MFPF assesses luminescence lifetime by modulation of light excitation frequency where the oxygen dependent phase shift of the emission is detected. Lifetime is related to phase shift by the equation: $\tau = \frac{\tan(\theta)}{2\pi f}$, where τ is calculated lifetime in s, f is LED modulation frequency in Hz, and θ is phase shift measured by the instrument. The signals are transmitted via connected glass fibre cable to the MFPF server (NeoFox®, OceanOptics, Dundin, USA) with an integrated light emitting diode, as well as temperature and atmospheric pressure transducers. An external thermistor probe compensates for temperature changes (once a multi-point temperature calibration is performed). Lifetime data were logged by NeoFox® Software (OceanOptics, Dunedin, USA) for calculation of absolute P_{O₂} values. Absolute P_{O₂} values, luminescence phase shift, luminescence intensity, temperature and ambient pressure were displayed at a digital sampling rate of 10 Hz.

Calibration of the FOXY-AL300 Oxygen Probe

P_{O₂} probes were calibrated at different oxygen levels and temperatures in a closed thermostat controlled gas-tight chamber according to the manufacturer's instructions. The chamber was purged with pure nitrogen (P_{O₂} = 0 mmHg), compressed air

(P_{O₂} = 158 mmHg) and pure oxygen (P_{O₂} = 750 mmHg), respectively, in consideration of atmospheric pressure with a fixed laminar flow of 2 L min⁻¹ at 20, 30 and 40°C. After stabilisation, the corresponding lifetimes were used to create a multi-temperature calibration table.

Ethics statement

This study was carried out in strict accordance with the recommendations in the Guide for the Care and Use of Laboratory Animals of the National Institute of Health. The protocol was approved by the Animal State Care and Use Committee of the Rhineland Palatinate, Germany (Permit Number: G07-10-013). All surgery was performed under deep anaesthesia, and all efforts were made to minimise suffering [15]. Animal experiments were performed at the Department of Anesthesiology, Medical Center of the Johannes Gutenberg-University, Mainz, Germany and laboratory experiments at the Department of Anesthesiology and Pain Therapy, Inselspital, Bern University Hospital, and University of Bern, Switzerland.

MFPF Validation *in vitro* using a porcine lung model

Eight piglets, *Sus scrofa domestica* (20 ± 2 kg), were investigated. After the induction of anaesthesia with a bolus of fentanyl 5 μg kg⁻¹ i.v., propofol 2 mg kg⁻¹ i.v. and single shot atracurium 0.5 mg kg⁻¹ i.v. via an ear vein, the pigs were orotracheally intubated (ID 8.0 mm cuffed tubing) and ventilated in pressure-controlled mode (AVEA, Viasis Healthcare, Höchberg, Germany). Vascular access was achieved by surgical cut down for the placement of an arterial blood pressure line in the femoral artery. Normocapnia (P_{aCO₂} 35–45 mmHg) was maintained with a tidal volume of 6–8 ml kg⁻¹ BW⁻¹. Anaesthesia was maintained by continuous infusion of fentanyl (5 μg kg⁻¹ h⁻¹ i.v.) and propofol (5–10 mg kg⁻¹ h⁻¹ i.v.). During the experiment, F_{IO₂} was adjusted (0.21, 0.4, 0.6, 0.8 and 1.0) to obtain P_{O₂} readings over the whole normobaric measurement range. Core temperature by rectal probe was maintained within the physiologic range (37.0–38.5°C) using a heating blanket.

Blood samples (10 ml each) were withdrawn at each F_{IO₂} level into heparinised gas tight syringes covered with opaque tape. For each sample, the tips of two FOXY-AL300 probes (OceanOptics, Dunedin, USA) were placed into the syringe outlet sealed with a rubber port to avoid air contact. After reaching steady state values, both MFPF-P_{O₂} readings were simultaneously recorded for 2 min using the corresponding animal core temperature for the measurement. Then, the same blood sample was analysed by conventional polarographic Clark-type electrodes (RapidLab 415, BayerHealthcare, Leverkusen) immediately afterwards.

MFPF validation *ex vivo* using an artificial circulatory setup

In order to provide standardised conditions and to simulate *in vivo* conditions, an artificial circulatory system was set up. The apparatus was built of: a) two oxygenators (Jostra Quadrox D, Maquet Cardiopulmonary AG, Hirrlingen, Germany), b) 3/8 inch silicon tubing (Fumedica, Muri, Switzerland) with 3/8–3/8 inch connecting pieces (Luerlock, Fumedica, Muri, Switzerland), c) two multi-flow roller pumps (Stöckert, Munich, Germany), d) a heat exchanger (HCU-30, Maquet Cardiopulmonary AG, Hirrlingen, Germany) and e) an ambient light protected measurement chamber (Figure 1). A switch valve between two independent closed circuits enabled the induction of a step change between highly oxygenated blood (F_{IO₂} 1.0, circuit 1) to oxygen free blood

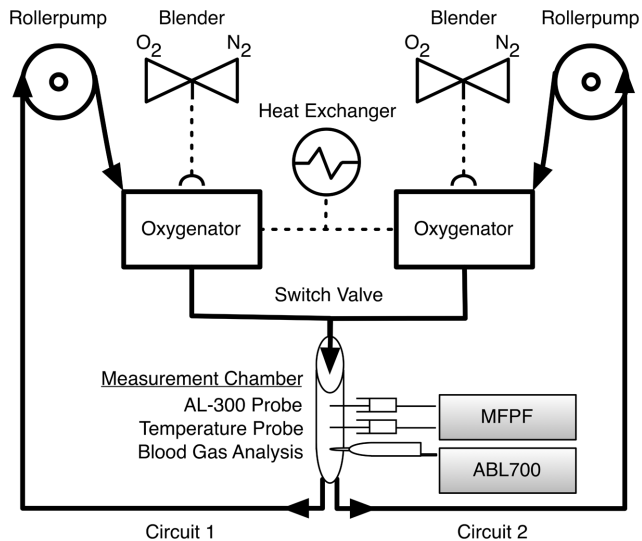


Figure 1. Artificial Circulatory Setup. Artificial circulatory setup with two independent circuits filled with human packed red blood cells (haematocrit of 30%). A switching valve between the circuits enabled a step-change between highly oxygenated (circuit 1: purged with pure oxygen) and oxygen free blood (circuit 2: purged with nitrogen). Black arrows represent direction of blood flow. Adapting the settings of the rollerpumps and the heating-cooling device (heat exchanger) allowed blood-flow and temperature to be controlled. Via the O₂/N₂ blenders, oxygen content could be adapted at fixed sweep gas flow over the oxygenators. Measurement chamber contained 1.) ports for insertion of MFPP probes (Foxy-AL 300); 2.) a temperature probe and 3.) a sampling port for Clark-typed based (CTE) P_{O2} analysis (ABL 700). doi:10.1371/journal.pone.0060591.g001

(F_{IO2} 0.0, circuit 2) in order to assess the time constants of the FOXY-AL300 probes in blood-phase.

The artificial circulatory system was primed with a mixture of crystalloid, colloid and human packed red cells to achieve a haematocrit of 30% and electrolyte values within the physiological limits. This setup allowed for control and variation of blood flow (by variation of rpm at the rollerpumps), temperature (by variation at the membrane equilibrator) and oxygen content (by P_{O2} variation at the blender).

In order to get measurements over the normobaric measurement range for the validation of MFPP against Clark-type electrode P_{O2}, F_{IO2} was set at random according to a computer generated list [16] from 0.0 to 1.0. To achieve an F_{IO2} of less than 0.21, a mixture of oxygen and nitrogen was used. For all measurements, duplicate MFPP P_{O2} readings (2 FOXY-AL300 probes) were recorded for 1 min duration alongside blood withdrawal for conventional polarographic Clark-type electrode P_{O2} analysis (ABL 700, Radiometer, Copenhagen, Denmark).

Measurements were performed according to the following protocols:

- 1) To assess the agreement of MFPP vs. Clark-type electrode P_{O2} at physiological body temperature conditions: at a temperature of 37°C, blood flow of 1.6 L min⁻¹ and a sweep gas flow of 1 L min⁻¹; 55 measurements were performed at varying P_{O2} levels.
- 2) To assess the impact of temperature: at a blood flow of 0.5 L min⁻¹ and sweep gas flow 0.5 L min⁻¹, temperature was set at random according to a computer generated list [16] to 20, 30 or 40°C. For each temperature level, 15 measurements were performed at varying P_{O2} levels.

- 3) To assess the impact of blood flow: at a temperature of 37°C and a sweep gas flow of 2 L min⁻¹, blood flow was set at random according to a computer generated list [16] to 0.8, 1.6, 2.4, 3.2 and 4.0 L min⁻¹. For each blood flow level, 10 measurements were performed at varying P_{O2} levels.

Statistical Analysis

Descriptive and statistical data analysis was performed using SPSS® V.19 (IBM Inc., New York, USA). For metric variables, statistical measures such as mean and standard deviation (mean±SD) were calculated. Linear regression analysis upon P_{O2} values measured by MFPP and CTE were performed. Bias and precision values were calculated by the Bland-Altman method [17,18]. The comparability was presented in explorative manner by description of mean differences, range of differences and 1.96-SD limits (lower and upper limit of agreement) [19]. In addition, linear regression analysis of difference versus mean was performed and then tested, if the slope is significantly different from zero. Furthermore, intra-class correlation between the two MFPP probes was assessed. To test the influence of blood flow and temperature variation, a multiple linear regression model was fitted: magnitude of P_{O2} measurements [(CTE+MFPP)/2], temperature and blood flow as independent variables; differences of MFPP and CTE as dependent variable. The categories of temperature and blood flow were handled with dummy coding. The analyses of data were done in explorative manner and the outcome of a statistical test with a *P*-value<0.05 was interpreted as statistically significant.

Results

MFPP Validation *in vitro* using a porcine lung model

Replicated porcine blood sampling revealed 80 duplicate MFPP-P_{O2} readings (range 63 to 749 mmHg) with the corresponding CTE samples (range 43 to 712 mmHg). The linear regression was described by the equation CTE = 15.59+1.18*MFPP (R² = 0.93; *P*<0.0001) (Figure 2A). Agreement by Bland Altman analysis showed a mean difference (mean_{diff}) in P_{O2} between CTE and MFPP of 69.2±64.1 mmHg (Figure 2B). The differences ranged from -50.1 to 215.6 mmHg within the 1.96-SD limits (lower limit -56.3, upper limit 194.8 mmHg). Linear regression of the difference versus mean showed CTE-MFPP = -0.64+0.20*[(CTE+MFPP)/2] (R² = 0.36, slope significantly different from zero: *P*<0.0001). Intra-class correlation between the two MFPP probes showed a reproducibility of R² = 0.98.

MFPP validation *ex vivo* in artificial circulatory setup

In artificial circulatory setup, MFPP-P_{O2} measurements ranged from 20 to 567 mmHg and the corresponding CTE samples from 11 to 575 mmHg. Linear regression yielded the equation: CTE = -8.73+1.05*MFPP (R² = 0.99; *P*<0.0001) (Figure 3A). Bland-Altman analysis calculated a mean difference (mean_{diff}) between CTE and MFPP P_{O2} measurements of 6.6±9.8 mmHg. Differences ranged from -9.7 to 20.5 mmHg within the 1.96-SD limits (lower limit -12.7, upper limit 25.8 mmHg) (Figure 3B). Linear regression of the difference versus mean showed CTE-MFPP = -8.62+0.05*[(CTE+MFPP)/2] (R² = 0.78, slope significantly different from zero: *P*<0.0001). Linear regression in a subset of P_{O2} between 0 and 140 mmHg yielded CTE = -7.84+1.13*MFPP (R² = 0.99; *P*<0.0001) (Figure 4A). Bland-Altman analysis of this sub-analysis showed a mean difference of 1.7±4.9 mmHg (Figure 4B). The differences ranged

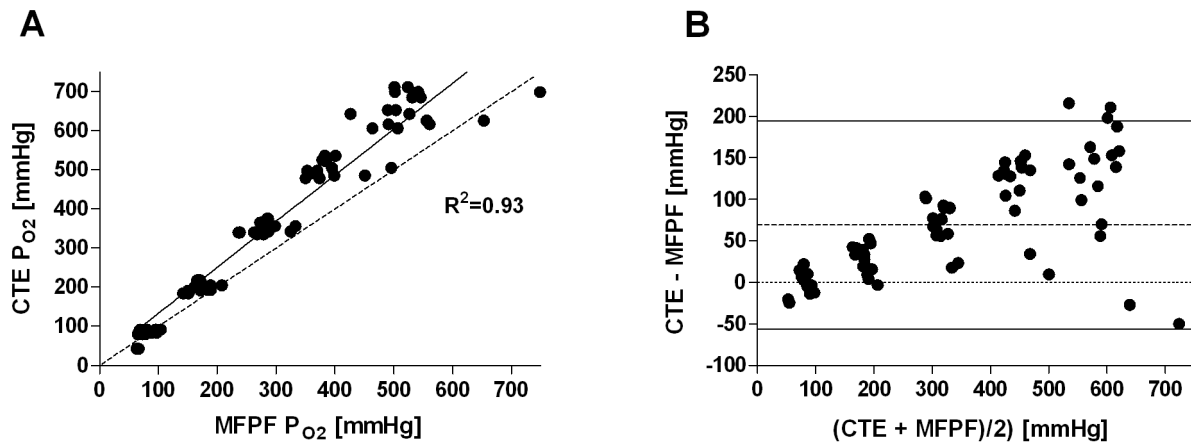


Figure 2. Multi Frequency Phase Fluorimetry P_{O2} vs. Clark-type Electrode P_{O2} (porcine blood *in vitro*, normobaric range). Panel A: Linear regression plot, the solid line displays the line of best fit, the dashed line shows the line of identity; Panel B: Bland-Altman plot showing the differences (CTE-MFPP) versus the means for absolute P_{O2} values. The dashed line represents the bias, the solid lines the 1.96 standard deviation interval.

doi:10.1371/journal.pone.0060591.g002

from -7.8 to 8.1 mmHg within the 1.96-SD limits (lower limit -8.0 , upper limit 11.4 mmHg). Linear regression of the difference versus mean yielded $\text{CTE-MFPP} = -7.47 + 0.13 * [(\text{CTE} + \text{MFPP}) / 2]$ ($R^2 = 0.84$, slope significantly different from zero: $P < 0.0001$). In total, reproducibility of $R^2 = 0.99$ between the two MFPP probes (intra-class correlation) was depicted.

Impact of temperature and blood flow on MFPP P_{O2} measurements

The influence of the temperature upon the differences of CTE and MFPP P_{O2} measurements reached from -0.6 mmHg (temperature = 20°C) to 31.8 mmHg (temperature = 40°C) (Table 1). The influence of blood flow on difference in P_{O2} of the two methods reached from 0.6 mmHg (blood flow = 1.6 L min^{-1}) to 14.8 mmHg (blood flow = 0.8 L min^{-1}) (Table 1). The linear regression model with the magnitude of P_{O2} measurements $[(\text{CTE} + \text{MFPP}) / 2]$, temperature and blood flow as independent variables showed a significant influence upon the magnitude of

P_{O2} measurements and a non-significant influence of temperature or blood flow upon the differences of P_{O2} measurements (dependent variable) (Table 2).

MFPP FOXY-AL300 Response Time

MFPP in combination with the uncoated FOXY-AL300 probes showed a mean response time of 1.48 ± 0.26 s in gas-phase and 1.51 ± 0.20 s in blood-phase after a step-change from pure oxygen (P_{O2} = 749 mmHg) to pure nitrogen (P_{O2} = 0 mmHg) at a digital sampling rate of 10 Hz (Figure 5). The monoexponential response time by Boltzmann fitting represents the time it takes the system to reach 63.2% of its final asymptotic value.

Discussion

Findings demonstrate MFPP technology's capacity for detecting changes in P_{O2} compared to Clark-type electrode (CTE) based P_{O2} measurements. For discrete samples, *in vitro* porcine blood

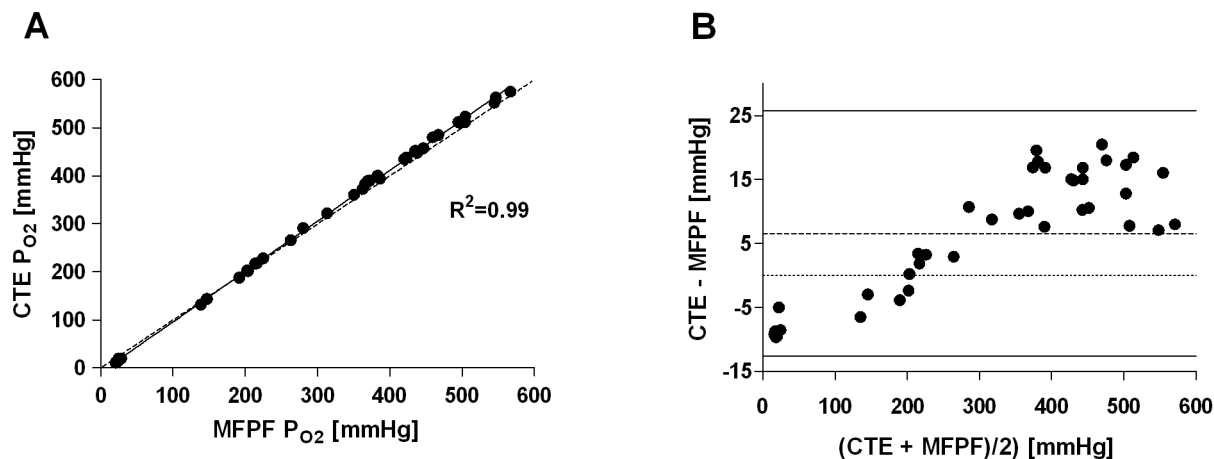


Figure 3. Multi Frequency Phase Fluorimetry P_{O2} vs. Clark-type Electrode P_{O2} (human blood *ex vivo*, normobaric range). Panel A: Linear regression plot, the solid line displays the line of best fit, the dashed line shows the line of identity; Panel B: Bland-Altman plot showing the differences (CTE-MFPP) versus the means for absolute P_{O2} values. The dashed line represents the bias, the solid lines the 1.96 standard deviation interval.

doi:10.1371/journal.pone.0060591.g003

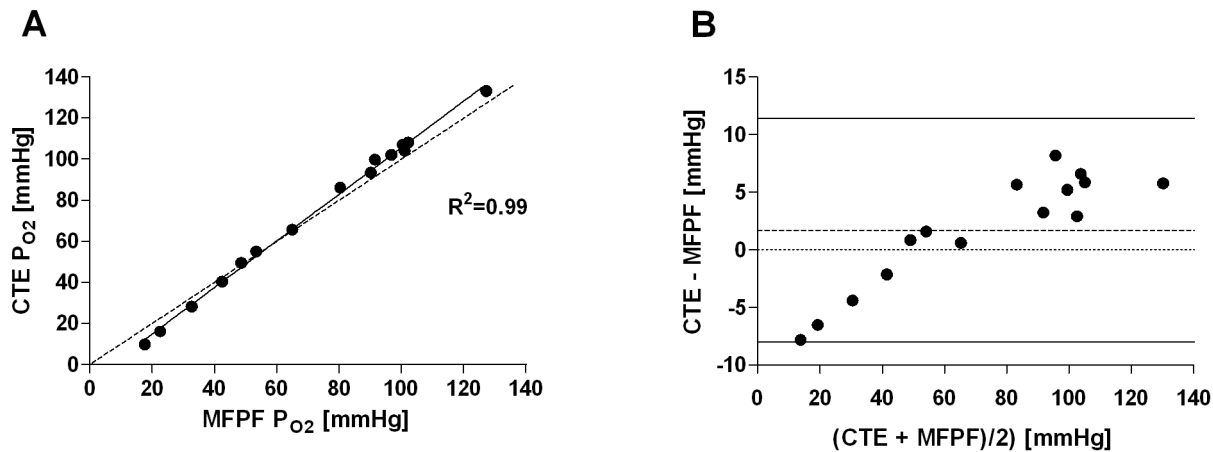


Figure 4. Multi Frequency Phase Fluorimetry P_{O2} vs. Clark-type Electrode P_{O2} (human blood *ex vivo*, hypoxic and normoxic range). Panel A: Linear regression plot, the solid line displays the line of best fit, the dashed line shows the line of identity; Panel B: Bland-Altman plot showing the differences (CTE-MFPF) versus the means for absolute P_{O2} values. The dashed line represents the bias, the solid lines the 1.96 standard deviation interval.
doi:10.1371/journal.pone.0060591.g004

phase measurements ($R^2 = 0.93$) did not give very tight limits of agreement. However, this study was not designed to validate MFPF as replacement for traditional *in vitro* blood gas analysis. For such a setup, we would have needed a configuration where the sensor and sample are part of a heated block with very tight control of both probe and blood sample temperature. The authors want to point out that the real application of MFPF is for flowing blood when the probe is placed *in vivo* - which was investigated by *ex vivo* measurements in an artificial circulatory setup filled with human blood. These findings demonstrate that MFPF technology provides high accuracy for P_{O2} measurements compared to CTE based P_{O2} measurements ($R^2 = 0.99$). The *ex vivo* measurements showed that MFPF technology accurately compensates for variation in temperature and that P_{O2} measurements are not

affected by variation in blood flow. MFPF response time in combination with the indwelling FOXY-AL300 probes was 1.48 ± 0.26 s in the gas-phase and 1.51 ± 0.20 s in the blood-phase (step-change from pure oxygen to pure nitrogen).

In summary, MFPF technology allows for fast, accurate and valid P_{O2} readings over the normobaric P_{O2} range (0–749 mmHg) for *ex vivo* experiments, as MFPF P_{O2} measurements ranged between 11 and 749 mmHg. This fact is the most important, as novel oxygen sensing technologies should be validated over the whole measurement range.

The *in vitro* animal model (porcine blood) showed good correlation ($R^2 = 0.93$), although the data was determined in clusters of oxygen concentration ($F_{I_{O_2}}$ 0.21, 0.4, 0.6, 0.8, 1.0). The observed high bias with positive drift as well as the enlarged

Table 1. Influence of temperature and blood flow on MFPF P_{O2} measurements.

	P _{O2} range [mmHg]	N	MFPF-CTE mean	MFPF-CTE SD	MFPF-CTE median
Temperature [°C]					
20.0	0–140	5	−0.6	4.6	0.9
30.0	0–140	5	0.4	5.9	0.6
40.0	0–140	5	5.3	2.4	5.8
Total		15	1.7	5	2.9
20.0	140–600	12	13.3	28.7	28.6
30.0	140–600	11	29.4	34.9	35.9
40.0	140–600	11	31.8	21.9	40.1
Total		34	24.5	29.4	29.3
Flow [L min^{−1}]					
0.80	0–600	9	14.8	4.5	17.3
1.60	0–600	7	.6	9.7	−2.4
2.40	0–600	8	5.4	10.5	8.6
3.20	0–600	7	6.5	10.1	10.1
4.00	0–600	9	4.1	9.4	7.1
Total		40	6.6	9.8	8.4

P_{O2} = oxygen partial pressure [mmHg]; MFPF = Multi Frequency Phase Fluorimetry; CTE = Clark-type electrode; SD = standard deviation.
doi:10.1371/journal.pone.0060591.t001

Table 2. Influence of temperature and blood flow on MFPP P_{O₂} measurements: Linear regression model.

Independent variable	Non-standardized coefficients			95.0% CI	
	Regression coefficient	Standard error	P-value	lower limit	upper limit
Temperature (base 20 °C)					
Constant	-2.335	10.483	0.825	-23.744	19.074
P _{O₂} -magnitude [(MFPP + CTE)/2]	0.062	0.027	0.031	0.006	0.118
30°C	12.854	11.466	0.271	-10.563	36.271
40°C	19.635	11.392	0.095	-3.629	42.9
Blood flow (base 0.8 L min⁻¹)					
Constant	-4.707	2.401	0.058	-9.586	0.171
P _{O₂} -magnitude [(MFPP + CTE)/2]	0.045	0.004	<0.001	0.037	0.054
1.6 L min ⁻¹	-4.461	2.441	0.076	-9.422	0.5
2.4 L min ⁻¹	-2.822	2.262	0.221	-7.42	1.776
3.2 L min ⁻¹	-2.093	2.328	0.375	-6.825	2.638
4.0 L min ⁻¹	-5.188	2.171	0.023	-9.601	-0.776

Linear regression model: magnitude of P_{O₂} measurements, temperature and blood flow as independent variables, differences of P_{O₂} measurements as dependent variable. P_{O₂} = oxygen partial pressure; MFPP = Multi Frequency Phase Fluorimetry; CTE = Clark-type electrode; CI = confidence interval.
doi:10.1371/journal.pone.0060591.t002

standard deviation can be most likely explained by the systemic experimental error to use the animals' core temperature for the *in vitro* measurements. The main intention of this first series was to obtain readings without the influence of blood flow. Therefore, we focused on how to avoid air contact to the withdrawn blood and decided not to insert the temperature probe into the syringes. However, we did not expect such an impact of temperature, which presumably seems even more evident at high P_{O₂}-levels (Figure 2B). This finding can be explained by the underlying MFPP technology, as in fluorescent quenching, signal intensity increases at lower P_{O₂} values. To fully understand the observed discrepancy of the *in vitro* (porcine blood) and *ex vivo* (human blood) results, we evaluated the difference of animal core temperature and blood temperature in the syringes two minutes after withdrawal post hoc in one further animal and found an error range of 0.9 to 1.6°C in ten repeated measures. Nevertheless, in the interesting physiologically hypoxic and normoxic (0–

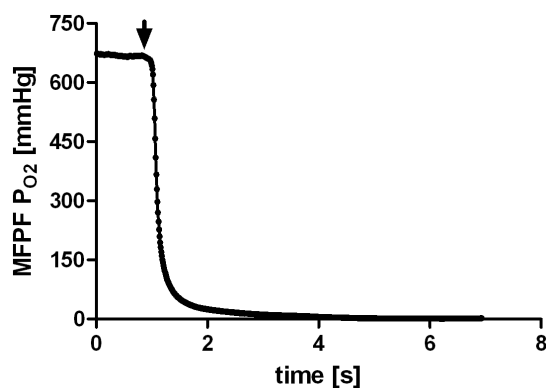


Figure 5. Multi Frequency Phase Fluorimetry/FOXY-AL300 Probe Response Time. Example of an MFPP step-down manoeuvre in artificial circulatory setup (human blood-phase). The graph displays the absolute MFPP P_{O₂} values over the time course. The arrow marks the time when the switching valve was changed between the oxygenated (750 mmHg) and non-oxygenated blood (0 mmHg) circuit.
doi:10.1371/journal.pone.0060591.g005

140 mmHg) P_{O₂} range, porcine results show that MFPP technology provides good agreement (Figure 2B) for discrete samples, although in our setup the technique was less accurate for high P_{O₂} values. Due to the underlying technological principle precision of MFPP, P_{O₂} values should increase within this physiologically interesting range (0–140 mmHg), which is supported by the present data. Thus, it seems unlikely that MFPP technology characteristics were responsible for this discrepancy, as intra-class correlation between the MFPP probes was extremely high (R² = 0.99) in porcine setup and MFPP measurements in the artificial circulatory setup (human blood) showed excellent agreement to CTE, even at high P_{O₂} levels. From our point of view, the porcine results nicely demonstrate the high temperature sensitivity of MFPP measurements and further highlight the importance of correct temperature acquisition. Instead of repeating this series, we decided to develop a new artificial circulatory system for further validation, where we could also investigate the influence of temperature and blood flow by standardised variation of these physiological values.

Under *ex vivo* conditions in the artificial circulatory setup (human blood), we found excellent correlation (R² = 0.99) of MFPP and CTE P_{O₂} with measurements equally distributed over the entire normobaric range (Figure 3). In general, MFPP values were slightly lower in comparison to CTE values. These findings were unexpected, as the MFPP technology, unlike polarography, does not consume any oxygen. These results might be explained by the fact that the blood-gas-analysers used allow a potential bias of 5% in calibration drift and it is well known that these are not really linear over the entire range. This underestimation decreases with lowered P_{O₂} values and is therefore of limited clinical importance (Figure 2, 3).

In general and as demonstrated by porcine results, temperature is obviously one major confounder on P_{O₂} measurement [20,21]. However, the present results of the artificial circulatory setup show that the MFPP technology accurately compensates for alterations in temperature if assessed strictly at the measurement site. This fact highlights the efficiency of multi-temperature compensation performed by MFPP software between 20 and 40°C. In this context, it would be desirable to have sensors available with an

integrated temperature thermistor to prevent errors such as temperature probe misplacement. In addition to temperature, blood flow may influence P_{O₂} measurements of an indwelling sensor [22]. The present *ex vivo* results confirm that MFPP technology correctly measures P_{O₂}, even under variations of blood flow within the range of 0.8 to 4.0 L min⁻¹.

One major advantage of MFPP P_{O₂} readings, next to high agreement and reproducibility, is high temporal resolution. We measured the monoexponential time constant for a step change in P_{O₂} at 1.5 s in blood. In contrast, the polarographic Licox probe showed response times up to several min [5,23]. Recently, faster P_{O₂} probes, such as the Neurovent PTO probe based on the fluorescent quenching of oxygen, have been presented. Although these probes reported higher response times (30 – 120 s), none of the commercially available technologies come near the temporal resolution of the uncoated ruthenium probe used in the current study [23,24,25,26,27,28].

The MFPP system is easy to set up and needs no complex calibration. In this validation study, the FOXY-AL300 probes were individually calibrated to minimise for potential errors, but in less demanding use, a calibration file supplied by the manufacturer for each probe can be used with acceptable accuracy. Furthermore, phase shift is not influenced by the medium the oxygen sensor is placed in, allowing simplified calibration in gas phase. Moreover, phase shift measurement is not influenced by the probe indicator dye concentration, photo bleaching of dye, or excitation source intensity. This results in stable signals with high signal to noise ratio [29].

Unfortunately, we could not obtain readings in a clinical setting in patients, as the indwelling probes available up to now (e.g. the FOXY AL-300) are not licensed for human application. Therefore, we investigated the MFPP technology *ex vivo* in a self-built artificial circulatory system filled with human blood. Although ruthenium-based dyes are commonly used in biological monitoring applications and are thought to be non-toxic, for future application in humans, the metallic surface of the probe and its tip containing ruthenium need to be coated with silicone or Teflon®.

References

- Clark LC Jr, Wolf R, Granger D, Taylor Z (1953) Continuous recording of blood oxygen tensions by polarography. *J Appl Physiol* 6: 189–193.
- Severinghaus JW (2002) The invention and development of blood gas analysis apparatus. *Anesthesiology* 97: 253–256.
- Hahn CE (1998) Electrochemical analysis of clinical blood-gases, gases and vapours. *Analyst* 123: 57R–86R.
- Kimmich HP, Kreuzer F, Spaan JG, Jank K, de Hemptinne J, et al. (1976) Monitoring of P_{O₂} in human blood. *Adv Exp Med Biol* 75: 33–40.
- Hoelper BM, Alessandri B, Heimann A, Behr R, Kempinski O (2005) Brain oxygen monitoring: *in vitro* accuracy, long-term drift and response-time of Licox- and Neurotrend sensors. *Acta Neurochir (Wien)* 147: 767–774; discussion 774.
- Purves MJ (1966) Fluctuations of arterial oxygen tension which have the same period as respiration. *Respir Physiol* 1: 281–296.
- Williams EM, Viale JP, Hamilton RM, McPeak H, Sutton L, et al. (2000) Within-breath arterial P_{O₂} oscillations in an experimental model of acute respiratory distress syndrome. *Br J Anaesth* 85: 456–459.
- Zaugg M, Lucchinetti E, Zalunardo MP, Zumstein S, Spahn DR, et al. (1998) Substantial changes in arterial blood gases during thoracoscopic surgery can be missed by conventional intermittent laboratory blood gas analyses. *Anesth Analg* 87: 647–653.
- Baumgardner JE, Markstaller K, Pfeiffer B, Doebrich M, Otto CM (2002) Effects of respiratory rate, plateau pressure, and positive end-expiratory pressure on PaO₂ oscillations after saline lavage. *Am J Respir Crit Care Med* 166: 1556–1562.
- Hartmann EK, Boehme S, Bentley A, Duenges B, Klein KU, et al. (2012) Influence of respiratory rate and end-expiratory pressure variation on cyclic alveolar recruitment in an experimental lung injury model. *Crit Care* 16: R8.
- Ganter M, Zollinger A (2003) Continuous intravascular blood gas monitoring: development, current techniques, and clinical use of a commercial device. *Br J Anaesth* 91: 397–407.
- Mahutte CK (1994) Continuous intra-arterial blood gas monitoring. *Intensive Care Med* 20: 85–86.
- Klein KU, Boehme S, Hartmann EK, Szczyrba M, David M, et al. (2011) A novel technique for monitoring of fast variations in brain oxygen tension using an uncoated fluorescence quenching probe (Foxy AL-300). *J Neurosurg Anesthesiol* 23: 341–346.
- Herveling A, Karmrodt J, Stepniak A, Fein A, Baumgardner JE, et al. (2005) A novel technique to follow fast PaO₂ variations during experimental CPR. *Resuscitation* 65: 71–78.
- Kilkenny C, Browne WJ, Cuthill IC, Emerson M, Altman DG (2010) Improving bioscience research reporting: the ARRIVE guidelines for reporting animal research. *PLoS Biol* 8: e1000412.
- Urbaniak GC, Plous S (2010) Research Randomizer (Version 3) [Computersoftware]. Research Randomizer website. Available: <http://randomizer.org>. Accessed 2013 Mar 4.
- Bland JM, Altman DG (1999) Measuring agreement in method comparison studies. *Stat Methods Med Res* 8: 135–160.
- Burkhardt H, Weiss C (2008) Evaluating influencing factors in estimation of renal function by extending the Bland-Altman approach. *Scand J Clin Lab Invest* 68: 171–176.
- Bland JM, Altman DG (1986) Statistical methods for assessing agreement between two methods of clinical measurement. *Lancet* 1: 307–310.
- Picandet V, Jeanneret S, Lavoie JP (2007) Effects of syringe type and storage temperature on results of blood gas analysis in arterial blood of horses. *J Vet Intern Med* 21: 476–481.
- Madiedo G, Sciacca R, Hause L (1980) Air bubbles and temperature effect on blood gas analysis. *J Clin Pathol* 33: 864–867.
- Grundmann A, Lubbers DW (1992) Can the flow dependency of the polarographic P_{O₂} electrode be used to measure arterial PO₂ and local capillary flow transcutaneously? *Adv Exp Med Biol* 317: 213–219.
- Haitsma I, Rosenthal G, Morabito D, Rollins M, Maas AI, et al. (2008) In vitro comparison of two generations of Licox and Neurotrend catheters. *Acta Neurochir Suppl* 102: 197–202.

In contrast to a silicone probe coating, Teflon® would allow for more rapid diffusion of oxygen and thereby maintain ultrafast probe response time. The challenge for the sensor engineering community will be to avoid direct contact of the fluorescent dye to blood components. Also, it is necessary to avoid protein adsorption and blood clotting to maintain signal stability and accuracy. Therefore, an intensive research effort is still necessary, but if engineering is to advance from laboratory-based research to commercial production levels, the MFPP technique could provide clinicians with an effective tool.

A limitation of the study is that we did not explicitly investigate the measurement stability over time. However, the present findings showed no calibration drift of the probes.

In summary we conclude that *ex vivo* MFPP-P_{O₂} readings are reproducible, and show excellent correlation and high agreement with the gold standard Clark-type electrode (CTE)-based P_{O₂} analysis. This novel technology adequately compensates for changes in temperature and allows for accurate measurements at various blood flow states. This feasible, accurate and easy to calibrate method has the potential to dynamically follow changes in blood oxygenation under various physiologic and pathophysiologic conditions with a high temporal resolution.

Acknowledgments

O. Aeby and B. Bencivenga for construction of the measurement chamber used in the artificial circulatory system. Department of Cardiovascular Surgery, Swiss Cardiovascular Center, Bern University Hospital, Bern, Switzerland (Director and Chair Prof. Th. Carrel) for collaboration and support for the artificial circulatory setup. B. Röhrig (statistician) for support in data management, reviewing the analysis of the data and proof reading the respective paragraphs of the manuscript.

Author Contributions

Manuscript revision: KUK KM JEB. Conceived and designed the experiments: SB AV KM JEB. Performed the experiments: SB AV BD VH BM JC RB. Analyzed the data: SB AV VH KUK. Contributed reagents/materials/analysis tools: SB AV RB. Wrote the paper: SB AV.

24. Citerio G, Piper I, Cormio M, Galli D, Cazzaniga S, et al. (2004) Bench test assessment of the new Raumedica Neurovent-P ICP sensor: a technical report by the BrainIT group. *Acta Neurochir (Wien)* 146: 1221–1226.
25. Huschak G, Hoell T, Hohaus C, Kern C, Minkus Y, et al. (2009) Clinical evaluation of a new multi-parameter neuromonitoring device: measurement of brain tissue oxygen, brain temperature, and intracranial pressure. *J Neurosurg Anesthesiol* 21: 155–160.
26. Jaeger M, Soehle M, Meixensberger J (2005) Brain tissue oxygen (PtIO₂): a clinical comparison of two monitoring devices. *Acta Neurochir Suppl* 95: 79–81.
27. Orakcioglu B, Sakowitz OW, Neumann JO, Kentar MM, Unterberg A, et al. (2011) Evaluation of a novel brain tissue oxygenation probe in an experimental swine model. *Neurosurgery* 67: 1716–1722; discussion 1722–1713.
28. Stewart C, Haitsma I, Zador Z, Hemphill JC, 3rd, Morabito D, et al. (2008) The new Licox combined brain tissue oxygen and brain temperature monitor: assessment of in vitro accuracy and clinical experience in severe traumatic brain injury. *Neurosurgery* 63: 1159–1164; discussion 1164–1155.
29. Lakowicz JR (2008) *Principles of Fluorescence Spectroscopy*, Third Edition. *J Biomed Opt* 13.